



Advance Bio-Photon Analyzer

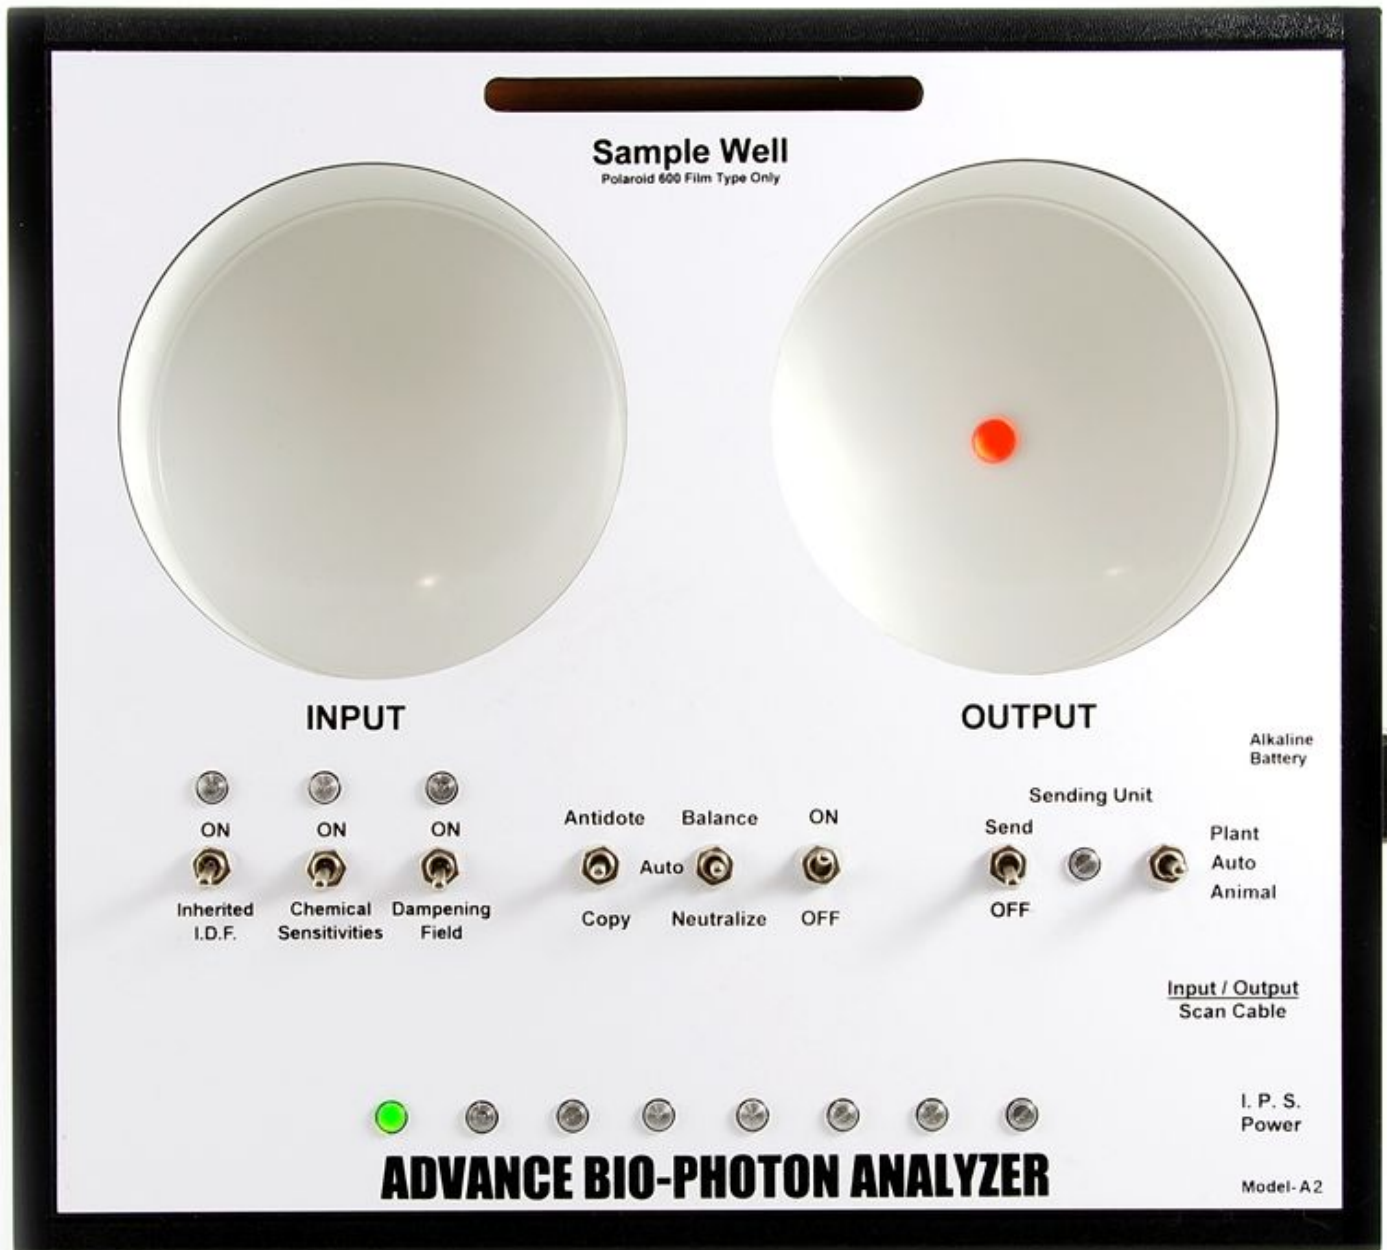

Model - A2

A2SRC.COM

Updated 2011

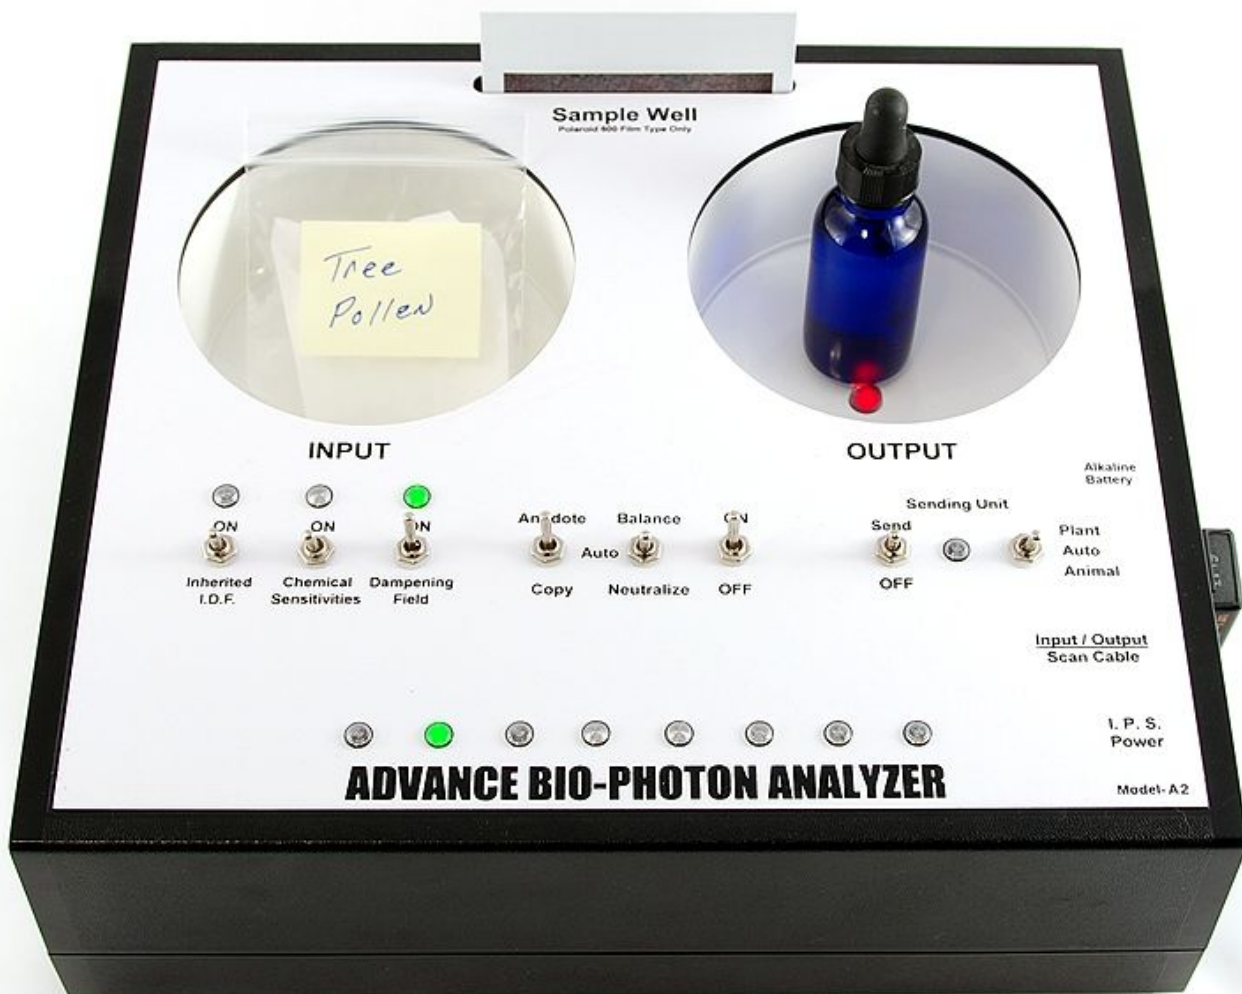


Model A2 Data Sheet

Advance Bio-Photon Analyzer

The Advance Bio-Photon Analyzer is one of the most advanced and sophisticated Isopathic generator ever made, while it remains the most simplest to use. The ABPA was developed for the chemical and allergy sensitive clients. The ABPA can make a self tuned custom Isopathic remedy in less than 40 seconds with a range of 0-cmm using intelligence auto potency internal software. The ABPA is the only instrument on the market that contains safety codes software that is both used in the A2 and transferred into the Isopathic media. Just think you now have an instrument that can make advance custom non-magnetic sensitive homeopathic remedies called Isopathic. No more trips to the store to find multiple remedies the ABPA can auto scan and find the best remedy and potency in just 40 second! And safe enough that a child can use, smart enough to figure how to remove energetic stress and stabilize you.

Q: Just ask you're self, what is my health worth to me??

A: Everything !!!!


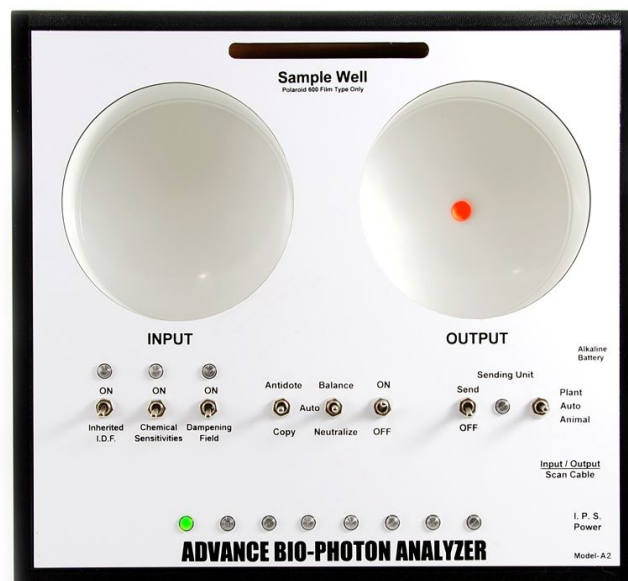


Features

- #1 instrument used to remove stress form the cellular system
- Used in many allergy eliminations protocols and techniques
- Self tuning to the users energetic system needs
- Auto Potency Range 0 – CMM (APR)
- Auto phasing range IN phase / OUT phase
- Isopathic safety codes design for chemical and energy sensitive
- Safety codes reduces the healing crisis reactions in many cases
- Portable power source runs on 9 VDC battery or AC wall adapter
- Can be used 24/7/365 to search and stabilize automatically
- Able to clean up food and other consumable product
- Creates Isopathic countermeasures that reduces stress on us
- Find internal/external weakness and energetically strengthens them
- Balances all energetic system so stress free harmony will work
- Goof proof, simple to uses
- 15 years of proven technology
- No need to buy expensive allergy vials, now make custom vials

Specifications

- Weight: 4.5 LBS.
- Size: 3 ¾" H, 11 1/2"W, 10 ¼ "D
- Switches: 8 Toggles
- Wells: 4" Input, 4" Output, Photograph
- Battery Power: 9 Volts Alkaline
- A/C Power: 12VDC @ 500 Ma a/c wall plug
- Plastic Type: ABS Plastic
- Scan Cable: 10' flex wrap cable
- Warranty: 3 Year Limited
- Drop resistance: 3 feet
- Software Knowledge: None needed
- Internal software: Proprietary Sealed
- Airport X-ray scans: Yes, Safe
- Isopathic fail: Strong Ultra Violet light ONLY



Why pay for expensive generic homeopathic vials when at the end of the day you may have used them only a few times. The ABPA will make custom designed Isopathic remedies to your subject. Perfectly tuned for there needs and includes the safety codes for additional protection to prevent healing crisis from occurring. Just think of it as your safety net! Once you use the ABPA you will wonder how you

TABLE OF CONTENTS

Pages	Items
	ABPA Model - A2
3	A2 Data Information Page
4	Table of Contents
5	Disclaimer
6	Manufactures Limited warranty coverage and exclusion
7	Dr. Alan W. Back Bio Page
8	Contents of your ABPA purchase
9	ANNA Procedure and Steps
10	ABPA A2 Top Ten Procedures
11	ABPA User Manual - Model A2
12	Accessories, Benefits, Components, Concepts, History
13	SIRM vs. Non SIRM, ANNA, Antidote - Auto - Copy, Balance - Auto - Neutralize
14	Biophoton, Books and reading, Boosting, Camera and Film Issues
15	Film issues and coming fixes
16	Cautions, Cellular Shock, Chemically-Sensitive's
17	Chemical - Sensitive's Switch, Chemical Toxins, Cleaning the ABPA, Common Sense,
18	Contents of your ABPA purchases, Copy Switch, Countermeasures, Dampening Field, Device Interface
19	Disarming, Energy Units, Environmental Contaminants, GV vs. RGV, Home / Office Detox
20	IDF Switch, Input Well, Output Well, Isopathic Remedy
21	Kinesiology Imprinting, Maintenance, Miasms, Minerals
22	Minerals, On/Off Switch, Option Switches, Output Well, Photo of a person, Photo of a animal
23	Photographic background, Photographic handling, Research Subject, Updates
24	Process Indicator LEDs, Safety Codes, Sampling Collections, Sample Collection, Objects, Sample Well
25	Sample to Avoid, Scan Cable, Sending Unit, SEND/ Off Switch, STRESS
26	Target Object, Warranty Exclusion, Wells
27	Blank page left for Notes
	AM3 Quick Start Guide
28	Special warning and Startups
29	AM3 Shipping Contents, Setting Up AM3 First Time Use
30	Steps 1 - Step 8
31	Steps 9 - Step 11, ANNA Knob and Setting
32	Step 12, Important Notes, Never Ever do this!!!
33	A2 information website to go to
34	AM3 New Mat information and handling sheet
35	Digital Media Interface (DMI) Information Flyer
36	Digital Media Interface (DMI) LAWS and startup steps
37	DMI Warranty page
38	A2 / AM3 Warranty page

DISCLAIMER

The information covered is to be used for educational and training purposes only.

The instrument CANNOT diagnose or indicate what problems are present or what treatments are need. Never wait or delay in seeing your certified health care professional for help.

This manual describes the Advance Bio-Photon Analyzer (A2) as a teaching tool to understand Intrinsic Data Fields (IDF). The ABPA is different form most scientific instruments, in that it operates in areas beyond the capability of traditional electromagnetic analyzers and spectrometers. IDF are informational fields and can occur with, or be superimposed upon, electromagnetic fields. IDF can also exist without electromagnetic fields.

The goal of this instrument is to reduce negative effects of stress from the environment which can overload the energy handling system of the body. At the same time, it is designed to increase the usable energy, improving the overall function and performance of the body's self-regulating mechanisms. Natural healing enthusiasts around the world use this strategy to maintain a healthy state for themselves, their families, and pets. We believe this cutting edge technology can help everyone to achieve a healthy edge for a healthy future.

The Advance Bio-Photon Analyzer (A2) uses subtle energy intrinsic data scanning technology to assess the imbalances of stress in the energy field only of the object scanned and will create an energetic Isopathic Countermeasure to remove stress from the energetic object only.

The APBA is a research device designed to investigate and influence the natural communication of these subtle energy data fields. Any perceived benefits which may be observed when using this equipment will be the direct result of improvements in the communication of the Inherited Data Fields within a subject or object and the effect these fields have on natural regulating mechanisms and/or the natural healing system.

Results may vary due to the unknown levels of stress present in each energetic object scanned.

The Advance Bio-Photon Analyzer (A2) is a therapeutic counter stress intrinsic instrument ONLY! These therapeutic intrinsic energies will help the energy field of the object to become more balanced. It will help remove energetic stress that may reduce the ideal function and performance of the energetic object in question.

If you wish to connect the Advance Bio-Photon Analyzer (A2 or AM3) to another instrument or outside equipment, ALWAYS check with us first at our website, www.A2SRC.com, to ask us to determine if it would be an approved device for use with the Advance Bio-Photon Analyzer (A2), and if a Device Interface Cable may be needed. The Advance Bio-Photon Analyzer (A2 or AM3) can usually be connected to 1) frequency generators, 2), sweep function generators, 3) Rife machines, and 4) frequency output devices, but ALWAYS check with us first. The Advance Bio-Photon Analyzer (A2 or AM3) should NEVER be connected to 1) radionics devices, 2) bio-scanner devices, 3) bio-sweep devices, or 4) orgone energy devices. Serious damage may result from such usage and the Manufacturer's Warranty will be voided if such a connection has been made.

Please use this Advance Bio-Photon Analyzer (A2) with the guidelines and boundaries set forth by this User Manual.

The Advance Bio-Photon Analyzer (A2) is NOT a Radionics or Scalar device of any type and should not be associated as one. If you have questions about the Advance Bio-Photon Analyze, please contact the Distributor from whom you purchased the instrument, or our website, www.A2SRC.com.

Always consult with your certified health care professional to verify that such equipment is right for you. Use only with the direction and guidance of your certified health care professional. Never use any instrument or device without checking first.

This is NOT a medical device by any means. The Advance Bio-Photon Analyzer (A2) works totally on the energetic stress body of the energy field of said object. ALL references are made in the relationship to the energy field of said object – NOT the physical body.

We make NO medical claims and do not support any medical treatments.

MANUFACTURER'S LIMITED WARRANTY COVERAGE

The A2 Service and Repair Center is the only authorized center to repair and reprogram the Advance Bio-Photon Analyzer (A2), Advance Matrix 3 System (AM3), and other products which Innovative Concepts produces. The A2 Service and Repair Center website is: www.A2SRC.com.

The Advance Bio-Photon Analyzer (A2) and Advance Bio-Photon Analyzer Advance Matrix 3 System (AM3) come with a 3-year Limited Warranty. This Limited Warranty covers the main unit and all other parts, including the International Power Supply Kit (IPS) and the 10' Scan Cable. This Limited Warranty covers switches, indicator lights, imprinter, wells, PCB, and the black plastic enclosure box. Repairs of such units may occur if needed. In some very few cases, the unit may need to be replaced, but this is only if deemed necessary by officials of Innovative Concepts.

All other products not mentioned above have a 1-year Limited Warranty. This will cover repair or limited replacement of said devices.

The user is responsible for shipping the unit to the A2 Service and Repair Center for repairs. After repairs are completed, the A2 Service and Repair Center will ship the unit back to the user and pay for shipping within the continental U.S. All other shipments coming from outside the U.S. must be arranged and finalized with the A2 Service and Repair Center before any work on the unit begins.

MANUFACTURER'S WARRANTY EXCLUSION

Warranty Exclusion may occur if the ABPA has been breached or tampered with. The ABPA (A2 and AM3) System uses tamper-proof screws and sets to protect the Wave Guide in the unit. The Wave Guide is a precision-tuned alignment device that is required for the Safety Codes to function. Without this Wave Guide, the Safety Codes may not function correctly. If the enclosure is opened or breached, the Wave Guide will be altered from the original factory setting. This will cause the unit to render a neutral safety function within the unit and corrupt the software so as to prevent downloading from occurring. If the A2 Service and Repair Center finds such tampering to alter, modify, or re-create the device, the Manufacturer's Warranty will be voided. The A2 Service and Repair Center will not repair or replace the unit.



Dr. Alan W. Back

Alan Back, N.D. is the creator of the Advance Bio-Photon Analyzer along several other Health recovery devices being used world wide. As child prodigy in electronics for 34 years along with his Military training in electronics which has helped to back up his years of research; He has dedicated his life to Research and Equipment Development in Energetic Sciences for the past 18 years. With his main focus on Allergy Elimination, body balancing in and Chemical Sensitive recovery. Consulting with numerous Health Practitioners to create new equipment, along with sittings on the board of Frequency Energetic Medicine with world class Doctors and Researches who are setting standards and practices in the field of Energetic Sciences. He is considered one of the world's authority and industries leader in the field of Energetic Sciences.

After being brought to his attention by his mentor Dr. Deloris Spence Chemical Sensitive people were some of Health Practitioners greatest challenges and growing in numbers. This was something that mainstream Medicine did not address due to their extreme energetic sensitivities. Dr. Spence proposed a challenged for him to find a way to help those stricken so they could regain their health and get their lives back by recovering them. Rising to the challenge led to the instrument known today as the A-2 (Advance Bio-Photon Analyzer) and the AM3 (Advance Bio-Photon Analyzer / Matrix 3 System) and with close to 35 different such medical devices he has created over his career and with years of research he has found it be extremely encouraging, not only did this instrument perform well on Chemical Sensitivities Clients recovery processes, but also helped on other health issues and challenges that faced Health Professionals on non-chemical sensitive clients with a wide range of applications on energetic levels through out the bodies systems.

Alan's development of cutting edge equipment has helped bring the Natural Health Professionals Practices out of the dark ages of treatments and therapies that were antiquated and mystical in nature into a more updated and modern therapies with electronic devices that have been proved to be more reliable. Using the knowledge gained in the U.S. Army as Technical Service for Special Operations Group specializing in Electronic and Non Conventional Warfare, serving both Overseas and Stateside gave him a leg up on the competition. Having wonderful success with his equipment over the years was not enough he soon enriched his person by attending Trinity College of Natural Health there he started to explore ways he could use his specialized training to help those who needed help so he went to work by obtaining the title of Doctor of Natural Health (N.D.) and C.N.H.P. (Certified Natural Health Professional).


Today along with his wife Dr. Misty Back and other college's he continues to work on new cutting edge equipment, therapies, educational seminars and consulting In his constant efforts to help everyone to gain the cutting edge with knowledge of treatment and recovery challenges available.

CONTENTS OF YOUR ABPA PURCHASE

- ◆ Advance Bio-Photon Analyzer – Model A2
- ◆ User Manual – what you're reading right now!
- ◆ International Power Supply Kit – with four adaptors for overseas use
- ◆ Scan Cable – 10 feet long, black, with a green LED at one end on the tip
- ◆ Top Ten Procedures - laminated
- ◆ Optional Items – additional accessories you may have ordered
- ◆ Disclaimer Information, Manufacturer's Limited Warranty Coverage, and Manufacturer's Warranty Exclusion
- ◆ Warranty Registration Sheet – please complete the information and return to A2 Service and Repair Center

Please open the shipping box carefully as contents may have shifted in transit. Make only a very shallow cut if using a box cutter. Please save the shipping box, as you will need to use the original shipping box for future service and possible upgrades.

Make sure all switches are either in the "OFF" or "AUTO" positions. Place the International Power Supply (used in all countries) into the Power Jack (located on the right side panel, in the lower left area), and plug the unit into the wall outlet.

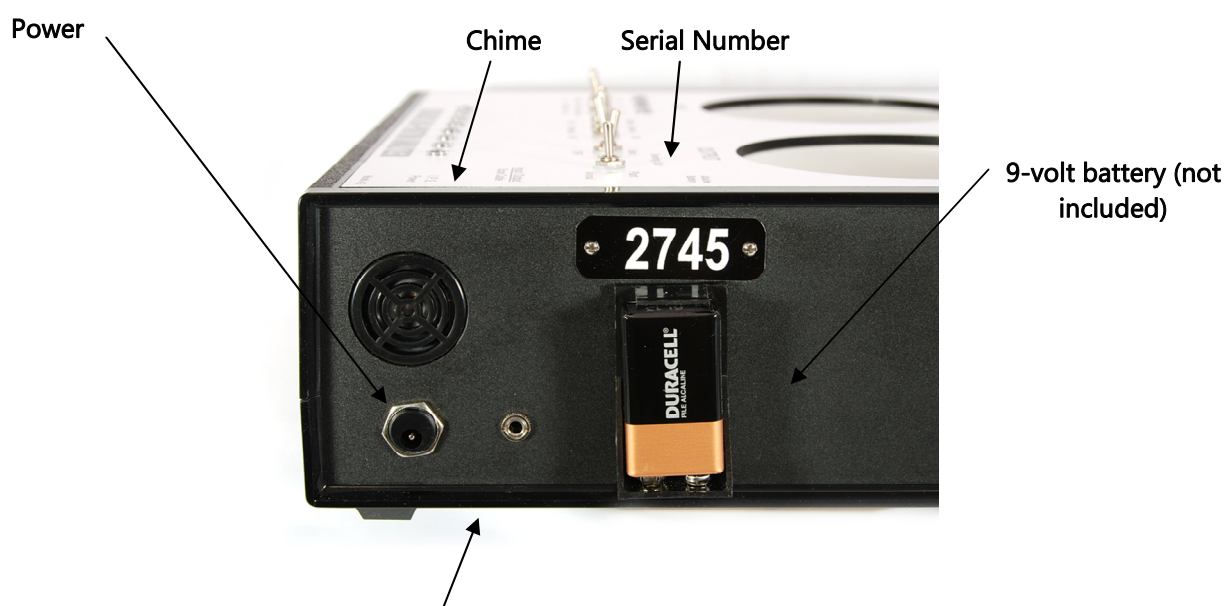

Bi-directional Port for LED Scan Cable, optional Device Interface Cable and other approved accessories

ANNA PROCEDURE

There is a method to follow in using the ABPA which makes a quick and easy matter of a sophisticated procedure. This method refers specifically to the settings of the Core Group toggle switches located in the center of the face of the ABPA. It is the most popular sequence used and the fastest way to achieve successful results with the instrument.

We will call it "ANNA", an acronym for


1) "ANtidote", 2) "Nutralize" + 3) "Auto", 4) "auto".

Inspect and clean wells before use. Place the sample object into the INPUT well, and/or the photograph into the SAMPLE well. Place the target object into the OUTPUT well.


1. "ANtidote": Place the left toggle switch in the "Antidote" position.
2. "Nutralize": Place the center toggle switch in the "Neutralize" position. "ON-OFF": Place the right toggle switch in the "ON" position. The ABPA will run the "Antidote"-**"Neutralize"** scan for 40 seconds (during which time the green LED lights at the bottom of the face of the ABPA will be on, each for five seconds in a sequence from left to right). At the end of 40 seconds of time, you will hear a ding-dong chime. This will be your signal to turn the right toggle switch to the "OFF" position.
3. "Auto": Place the left toggle switch in the "Auto" position.
4. "auto": Place the center toggle switch in the "Auto" position.

"ON-OFF": Place the right toggle switch in the "ON" position. The ABPA will run the "Auto"-**"Auto"** Isopathic Countermeasure for 40 seconds (during which time the green LED lights at the bottom of the face of the ABPA will be on, each for five seconds in a sequence from left to right). At the end of 40 seconds of time, you will hear a ding-dong chime. This will be your signal to turn the right toggle switch to the "OFF" position. This is the end of the ANNA procedure.

This ANNA procedure is the favorite among many users and researchers because it instructs the ABPA to scan the greatest amount of energetic patterns and sources of stress in the shortest period of time. As the ABPA scans these energetic patterns of the Research Subject, it creates what researchers call an Isopathic Remedy or Isopathic Countermeasure, designed to alleviate stress on the Research Subject. These are then transmitted in the form of vibrational patterns which can cover great distances.

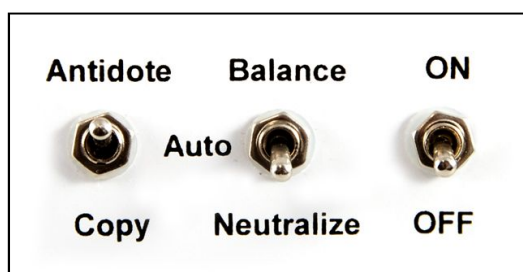

1) "ANtidote", 2) "Nutralize"

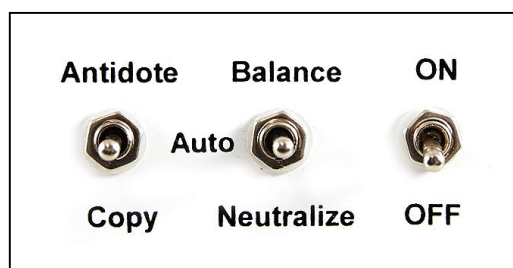


3) "Auto", 4) "auto"

ABPA A2 TOP TEN PROCEDURES

1. **Quick Fix Protocol** – Alan Back’s favorite daily balancing procedure. It takes about three minutes, and no photo is required. (The ABPA can perform this ANNA procedure without using a photo, without a biological sample, and without using a homeopathic remedy medium in the OUTPUT well.) Have the Research Subject place his or her fingertips of the left hand over the front edge of the INPUT well, and fingertips of the right hand over the front edge of the OUTPUT well, being careful that the fingertips do NOT touch the sides or bottoms of the wells. (Fingertips and fingernails are very strong emitters of photonic energies.) Run the ANNA procedure, turning the OFF-ON toggle switch while leaving both hands in both wells, and moving the toggle switch with the right thumb of the right hand. The 1-2 Step (aka Quick-Fix) is used 95% of the time. Standard ANNA Procedure is used for this procedure been previously referred to, casually, as the “1-2 Step”. And Alan Back personally recommends this about 95% of the time. In this Procedure, the Subject’s left hand is placed into the bottom half of the INPUT well (without letting the fingertips touch the bottom or the sides, although there is not a problem for the fingernails to touch the bottom). Scan Cable Use for Specific Areas of concern (tennis elbow, sore muscle) 24/7 Sending Unit
2. **Scan Cable Use for Food Clearing and Optimizing** - The ABPA Scan Cable is 10 feet long and plugs into the XXX on the side of the unit. The Scan Cable, like the INPUT well and OUTPUT well, should be kept meticulously clean. There are several ways the Scan Cable can be used. It can be wrapped around a bag of groceries. The ABPA by way of using the Scan Cable will search the food for allergens to the Subject and provide a counter-measure. Also, the Scan Cable can be wrapped around a part of the body, such as a wrist or knee, that will aid that part of the body that the Scan Cable is wrapped around. In grocery scan cable section - All foods are subject to toxic chemicals, many airborne, even if they are grown organically.
3. **Creating a Personalized Reagent Isopathic: See Isopathic**
4. **Creating a Generic Isopathic Imprint: See Imprints**
5. **ANNA into a bottle of drinking water** - Daily, do a scan each day, and neutralize into a bottle of drinking water to drink throughout the day.
6. **Environmental Detox using Coffee Filter** – You will need a blotter agent (such as a coffee filter) and a sealable plastic bag. Tack the coffee filter to a post or tree to collect outdoor contaminants for a week. Then it should be placed in a sealed plastic bag and labeled as to area, date, and location.
7. **Home and Office Detox** - (Broadcasting for “gunk” contamination indoors using adhesive tape and photo samples, and bottle of misting water) also vehicles, fields, herds. Touch tape where dust will gather. Do it for each room of the house. Do ANNA with each tape sample from each room and put it in one spritzer (or mister) bottle of water (or mister) and aim toward all four upper corners of room and center of ceiling of each room. Also from furnace vents and air intake vents, pet hair, The photograph becomes a representative sample of the room; the sample tape with the room’s contamination attached to it also becomes another sample of the room. Subjects who are very chemically-sensitive to their everyday indoor environment can easily and quickly make an Isopathic Counter-Measure following this procedure. Take a small (approximately six-ounce) plastic mister bottle and fill it half full of water. Take a piece of adhesive tape about 6” long and collect samples from furniture, walls, floorboards, trim boards, room décor items, curtains or window coverings, and carpet or floor coverings. Fold the tape in half with the sticky sides together and put the tape sample in a clean, sealed, small plastic bag. Label the bag with the date and location of the source of the tape sample (such as “office”, “living room”, “bedroom”, “bathroom”, “playroom”, etc.). Put the adhesive tape sample sealed inside a small plastic bag and place in the INPUT well. Use the
8. **Memory Mapping** - Take Subject photo, vial of half water and half alcohol in OUTPUT well, Auto, auto while in training mode (during the time she’s competing or training); write paragraph of information about her workout training; Workout #1, date; workout #2, date; use on any sport, high-performance workout; her workout was constantly being monitored by the ABPA and dumping it into vial to optimize performance to create stability; memorized what she was doing throughout course; machine turned on while she was working out; she documented; was gathering data on the athlete; take 2 or 3 best workouts of group of workouts, put in vials, keep running those
9. **To remove the energy of a previous homeowner: See Detox**
10. **Kinesiology Imprinting** - Kinesiology Imprinting; tooth:00:43:00 put index finger of right hand on the troubling tooth, or on the facial cheek area adjacent the troubling tooth. Place the fingertips or the index finger of the left hand into the INPUT well. Do not let the fingers touch the sides or bottom of INPUT well. Make an Isopathic Counter-Measure with water, alcohol, or glycerin.

ADVANCE BIO-PHOTON ANALYZER

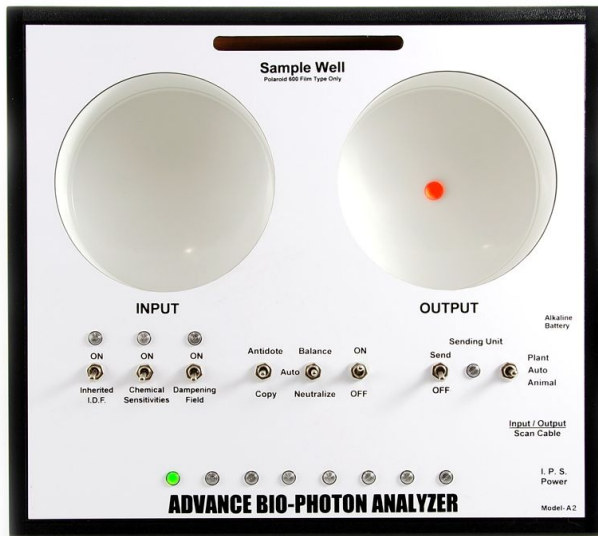

User Manual ABPA Model A2

Thank you for your purchase of the ABPA. The ABPA, an acronym for Advance Bio-Photon Analyzer Model A2, is of exceptional concept, design, and manufacture. It is easy to use. It has been accurately and precisely engineered – so it performs the way it was designed to perform. It is exclusive - there's no other instrument anywhere in the world that has been designed to do what this one does. Wow! What a concept!

We know that as a purchaser of the ABPA, you have already defined yourself as a forward-thinking, motivated individual who desires a life of vibrant health and well-being. We thank you and value your participation in joining us so we can all learn more about ways to apply this unique and exciting technology. This is a fun, effective, wonderful technology that we're all excited about. As a team, all of us join together in wishing you every success with the ABPA.


Our many environments are abuzz with many energetic systems, only some of which we can see (light), or hear (music), or feel (exhilarating negative ions following a refreshing storm). The ABPA is a unique and valuable resource to a quality life. It makes energetic patterns. If you would like to learn more about the research upon which the ABPA is based, you can learn a lot by looking at biophoton energy and a small sliver of science known as etherical theoretical quantum mechanics.

This User Manual has been prepared with the hope that you will find it helpful to better understand the ABPA and its intimate connection with biophoton energy technology. This information has been formatted so that you can remove your new ABPA directly from its packing box, read this User Manual, and begin using your ABPA immediately. This User Manual will make it easy for you to do that.

Throughout this User Manual, we will frequently use the words "Subject" and "Research Subject". This could mean living objects (such as human beings, dogs, cats, horses, pets, fish) or botanicals (such as plants, seeds, food, trees, yards, fields, farms, ranches) or non-living objects (such as rooms, homes, offices, vehicles, hot tubs, swimming pools). And you'll probably be able to think of more "Subjects" than we listed here!

After you have become familiar with the operation of the ABPA and have used it a while, if you have questions or feel you would like more information, or would like to have your ABPA software and hardware updated every year or two, please contact the ABPA Service and Repair Center at its website, www.A2SRC.com.

The ABPA cannot be used for harmful, negative, or detrimental purposes. There are Safety Codes built into the software of the ABPA so that it becomes ineffective if it is tampered with. Some of the concepts connected with the software are proprietary and known only to the inventor and engineer, Alan Back. Please join us in not asking him to divulge any of them – of course, we'd all like to know what they are, but let's be good-natured about it and don't ask!

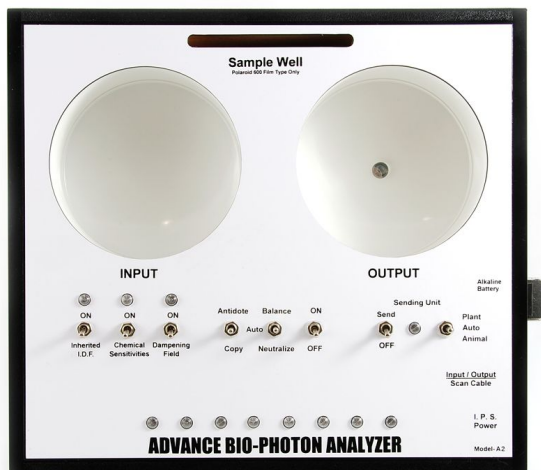

ABPA: The ABPA is a highly sophisticated, advanced instrument that detects subtle energy by scanning a Research Subject. It recognizes Energetic Patterns, then creates an Isopathic Countermeasure to assist recovery. The goal is to reduce the negative effects of various types of stress which can overload the energy handling system of the body. At the same time it is designed to increase the usable energy, improving the overall function and performance of the body's self-regulating mechanisms. Natural healing enthusiasts around the world use this strategy to maintain a healthy state for themselves, their families, and pets. There is no diagnosis. In fact, you don't even have to know what's wrong with the Research Subject.

ABPA ACCESSORIES: The Device Interface Cable interfaces the ABPA with other devices, such as computers, frequency generators (such as the GB-4000), and CD players (to be used with meditative CDs with frequencies encoded). The ABPA website, A2SRC.com, should be contacted first to ask about interfacing the ABPA with any other electronic devices. Should any damage occur to the ABPA without first checking with the Service and Repair Center, the Warranty for the ABPA could be invalidated.


ABPA BENEFITS: At any given point in time, the body believes it is in good health. Even though it may be going downhill fast, the body still believes it is in good health. The body does not have any reference or memory of what bad health is. It has no way to remember good health from bad health. What the ABPA does is re-teach the body what good health is, not just what the body believes good health is. Also, the ABPA can be used to enhance the viability and strength of seeds used for planting. It can augment germination rates and enhance growth. The ABPA can also adjust to what the Subject's body can accept continuously. The ABPA is an experimental device, not a medical device. If the Subject's recovery has begun but at various times reaches a plateau, use the "Quick-Fix" procedure found in the "Top Ten Procedures" instructions, from 1 to 5 times per day.

ABPA COMPONENTS: The ABPA is lightweight (about 3 pounds), small (11-1/2" by 10-1/2" by 4"), and durable. The casing is ABS Plastic (15%-35% Acrylonitrile, 5%-30% Butadiene, 40%-60% Styrene) which has very low emissions and is recognized for its minimal leeching properties. The white skin on the face of the ABPA is vinyl, durable to heat and cold, and resistant to ultraviolet light. All these things are very important to chemically-sensitive people.

ABPA CONCEPT IN A NUTSHELL: The design concept of the ABPA is that it scans the energetic field of a Subject. It also scans for stressors that may be compromising the health and vitality of the Subject. Once the stressors are recognized, they are analyzed. Then the ABPA selects electro-energetic Isopathic Countermeasures to offset the stressors, and transmits those Countermeasures to the Subject (regardless of the distance from the ABPA to the Subject). Wow! What a concept!

"Amid all the mysteries by which we are surrounded, nothing is more certain than that we are ever in the presence of an Infinite and Eternal Energy from which all things proceed."

-- Herbert Spender, writer and philosopher

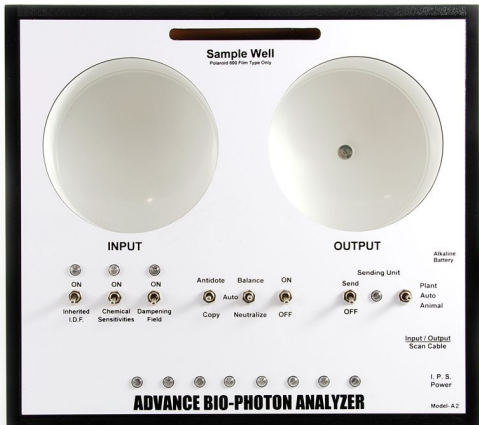


ABPA HISTORY: The ABPA was first developed in 1988 by Alan Back. Its several versions have been known as the "Advance Bio-Photon Analyzer", the "Clinical Bio-Photon Analyzer", the "Advance Unit", the "A1", and the "A2". It was originally developed for chemically-sensitive Subjects to help take the stress off their physical, energetic, and nervous systems. This technology is now being accepted by people who may have been skeptical about it in the past. It focuses on restoring the normal form and function of a Research Subject's subtle bio-electro-energetic system.

ABPA IS A NON-SIRM UNIT: The ABPA is a non-SIRM unit, meaning it is a non-Stress Induced Reagent Module.

ABPA IS NOT: The ABPA is not a radionics machine. It does not use scalar technology. It does not transmit Hz frequencies.


ANNA: These letters form an acronym for **AN**tidote, **N**eutralize + **A**uto, auto. They refer to the main procedure that can be easily memorized to complete a process of scanning a Subject (by way of photograph placed in the Sample Well or by way of biological sample placed in the INPUT Well) and then making an Isopathic Remedy or Countermeasure.


ANTIDOTE – AUTO – COPY SWITCH: This toggle switch set in the "Antidote" (upward) position is used exclusively to Antidote. It does not balance or copy. It Antidotes to create a remedy to counteract the energetic effects or patterns of poisons and toxins in the Subject. It scans for detrimental energy patterns which may be causing stress to the Research Subject.

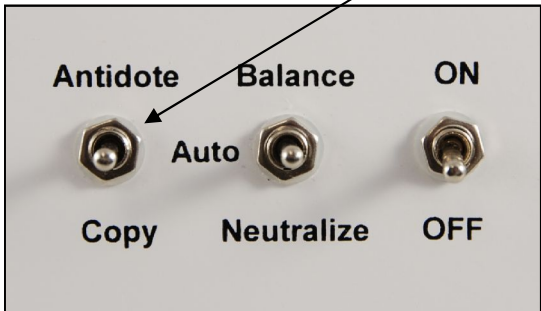

This toggle switch set in the "Auto" (center) position is used when there is no particular criteria for setting it in either the "Antidote" or "Copy" position. In the "Auto" position the unit will determine by itself what it needs to do to maintain balanced, etheric frequency patterns in the Research Subject. The ABPA will choose the best frequency patterns to send to the Research Subject based on its intelligent internal software. It will determine if the Research Subject is in a state of deficit or in a state of excess. If you are uncertain as to which position to set this toggle switch in, always select "Auto", and the ABPA will make its own decision.

This toggle switch set in the "Copy" (downward) position will copy resonant frequency patterns from one substance into another substance or Subject. This is especially useful for homeopathic practitioners who wish to copy the energy from one homeopathic substance to another. Some researchers have found this procedure helpful in order to copy food supplements, vitamins, minerals, and other nutrients. The percentage of any original substance that you can copy will vary with conditions which none of us understands. However, many practitioners are able to determine the amount of copying capability by using kinesiology, muscle testing, pendulum testing, or dowsing.

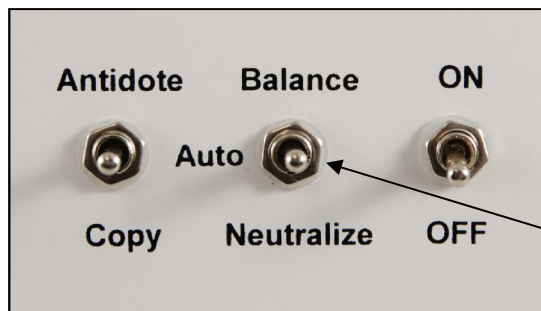

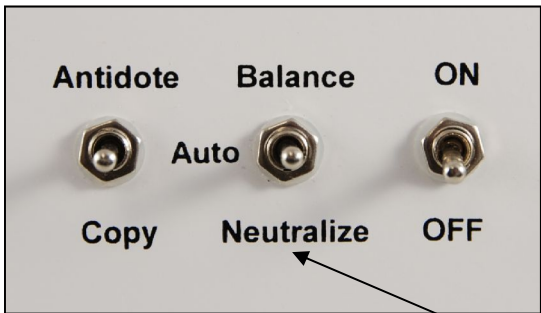

BALANCE – AUTO – NEUTRALIZE SWITCH: This toggle switch set in the “Balance” setting is used to bring the subject into a state of equilibrium and normal form and function. This is done by the application of a countermeasure designed to balance the subject’s energetic system or energy field. This concept of balance is especially useful if the conditions causing stress on the system are unknown. It simply assists to bring the subject into a general state of balance and well-being.

This toggle switch set in the “Auto” (center) position is helpful if the conditions causing the stress are unknown. In the “Auto” position the unit seeks to discover, by way of scanning, detrimental informational patterns which might be causing stress on the system. The ABPA continually monitors the balance point of the subject and determines the best energetic frequency patterns to transmit.


This toggle switch set in the “Neutralize” position scans the research subject for detrimental, unbalanced energetic patterns and transmits the appropriate countermeasure. The unit focuses its scanning capability specifically on detrimental informational fields in the subject and the subject’s immediate vicinity or nearby environment.



BIOPHOTONS: Biophotons, or ultraweak photon emissions of biological systems, are weak electromagnetic waves in the optical range of the spectrum – in other words: light. All living cells of plants, animals, and human beings emit biophotons which cannot be seen by the naked eye, but can be measured by special equipment developed by German researchers. This light emission is an expression of the functional state of the living organism and its measurement therefore can be used to assess this state. Biophoton energy is stored in the DNA molecules of the nuclei of cells of an organism. Researchers have learned that cells can actually communicate with each other, regardless of the physical distance between them.

BOOKS HELPFUL TO UNDERSTAND SUBTLE ENERGY RESEARCH WORK: “Vibrational Medicine: New Choices for Healing Ourselves” by Richard Gerber, M.D.; “The Body Electric: Electromagnetism and the Foundation of Life” by Robert O. Becker and Gary Selden; “Energy from the Vacuum” by Tom Bearden.

BOOSTING: Boosting can be done with herbs (such as ginseng, which is goof for the immune system) in bottles. You can create an isopathic remedy that is tuned specifically to your energetic body and then increase the potency of the remedy.

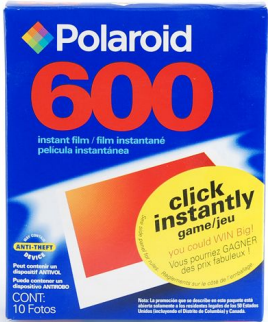

CAMERA AND FILM: The right camera to use is a Polaroid. The right film to use is Polaroid 600 Film (either Color, or Black and White) because it has the least amount of chemicals to create the image. Only Polaroid 600 Film should be used because the ABPA and its software have been calibrated to only that specific type of film. Polaroid 600 Film contains silver halide particles (which capture both the positive and negative images simultaneously) that are capable of storing the energetic representation of the Subject at the time the photograph is taken. There is a high silver halide emulsion in the layering of Polaroid 600 Film. Those silver particles are very energetic, and that energy can be picked up in the photograph of the

Polaroid Film 600

We are sorry to see the Polaroid 600 Film go,


There were many units and instruments that depended on the film to complete the Bio Feed back loop. The ABPA was one of those that needed the film. However when I made the instrument I gave the user other options to use if they did not have access to the film or if your subject was not willing to have a photograph taken like some Indian tribes and religious groups.

Please be aware there are many other types of film out in the world and **NON** of these will work with the A2/ AM3 units. The unit was special calibrated for just this P600 film. We are current producing the new Digital Media Interface (DMI) . This DMI will have that ability to hold the digital photographs (see DMI Laws page 36) .

After thinking about it for a long time I decided to leave the section about the Polaroid 600 film handling. It has come to my attention that there are still a few a very few that still have this 600 film. I will retire this section at the end of 2010 . At the time the DMI will have it's own section to cover the Photo coverage pages 35,36.


Contact your distributor for more information.

Dr Alan Back
Innovative Concepts
A2SRC.COM

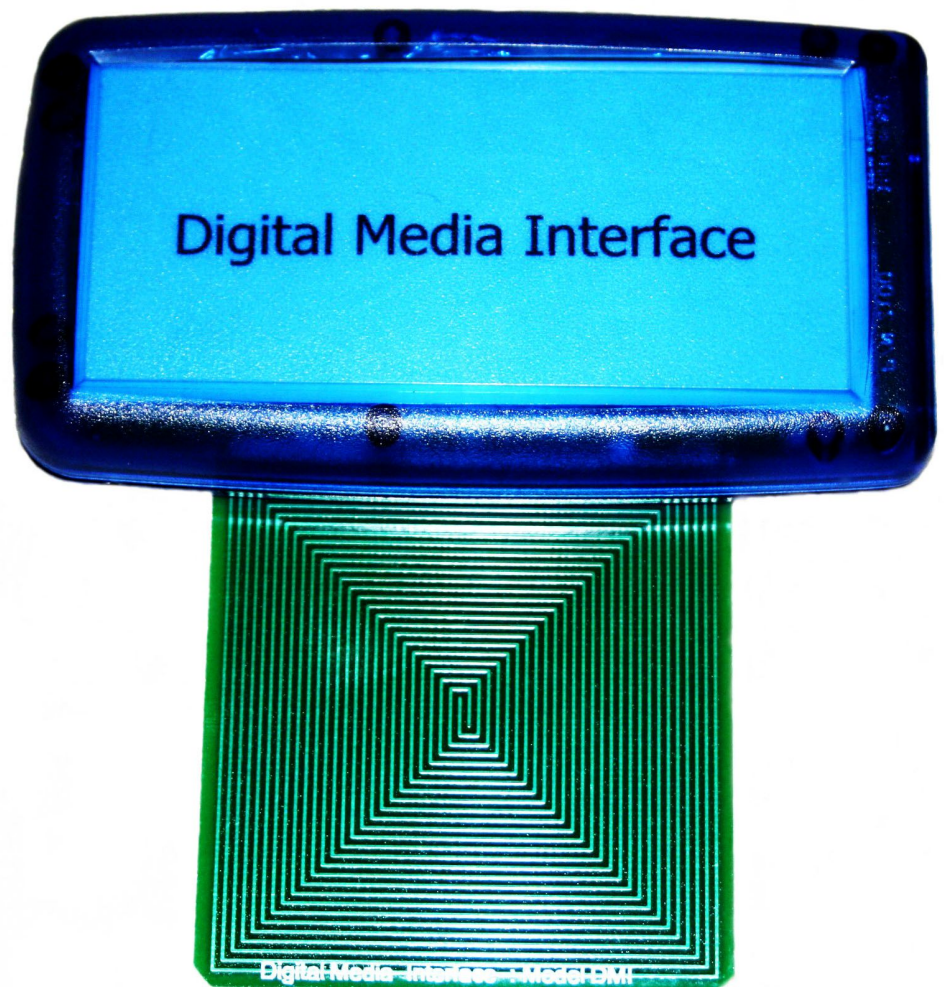

Research Subject by the ABPA. The ABPA has been calibrated to work from this film, and this film only.

CAUTIONS: Only use Polaroid 600 Film photographs in the Sample Well, as the ABPA has been calibrated with Safety Codes which provide a safety feedback loop. Do not use photographs taken with other films, such as from a digital camera printed on computer photo paper. The ABPA has not been programmed for use with other types of film and paper. Using any media other than Polaroid 600 Film will bypass the programmed Safety Codes and could produce undesirable results. Never turn the ABPA power off while a program is running. That the unit is running a program is indicated by any one of the eight green LED Indicator Lights located in a single row near the bottom of the face of the ABPA. Each light will be on for 5 seconds, for a total of 40 seconds. When running a program, the current operational status of the unit is indicated by a sequential lighting of the 8 LED Indicator Lights, each in turn, from left to right, for 5 seconds each. After the LED Indicator Light to the far right goes off, this indicates that a complete sequence is finished, and all lights will remain off for several seconds. THE UNIT SHOULD ONLY BE TURNED OFF WHEN THE FAR RIGHT LED INDICATOR LIGHT HAS GONE OFF, AND THERE IS A SLIGHT PAUSE BEFORE THE LED INDICATOR LIGHT SEQUENCE BEGINS AGAIN, FROM THE FAR LEFT.

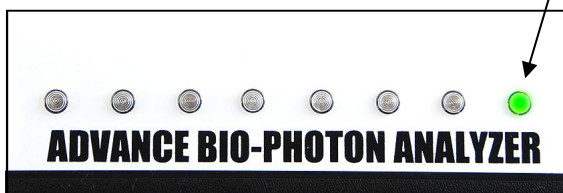


CELLULAR SHOCK: Some people can reach a condition in which they become nearly incapacitated and exhibit unusual symptoms that make it difficult to function effectively on a daily basis. Sometimes they can get into situations in which they appear to acquire great amounts of energy and operate with endorphin-excess. Literally, they're in shock and their bodies get locked up. Without the right key to unlock this cellular shock, a person can become exhausted via the Superman Effect. Sometimes there are high levels of residual deposits which have accumulated in their bodies that are similar to mineral deposits in the ground. Sometimes the slope becomes extremely steep, which indicates their reserves are being depleted. With some addictions, they appear to go through symptoms of withdrawal and their mental focus becomes clouded. There may be short, intermittent periods of time in which they can come out of cellular shock. In the ABPA software there are codes to look for cellular shock or remnants of cellular shock, determine what the pattern is, and the Countermeasure to take them out of cellular shock.

CHEMICALLY-SENSITIVE SUBJECTS: A chemically-sensitive Subject may only be able to tolerate 2 or 3 Energy Units of the total 20 Energy Units available through the ABPA. Therefore, the ABPA has been designed to recognize that chemical sensitivity in a Subject, and will reduce its own power output, often up to 80%. It will provide a very mild, very soft, very detailed scan of the Subject (which most chemically-sensitive people can easily relate to, and appreciate). The ABPA will engage more of the Safety Codes to benefit the Research Subject.

*"One-quarter of what you eat keeps you alive.
The other three-quarters keeps your doctor
Alive."*

(Hieroglyph found in an ancient Egyptian tomb.)

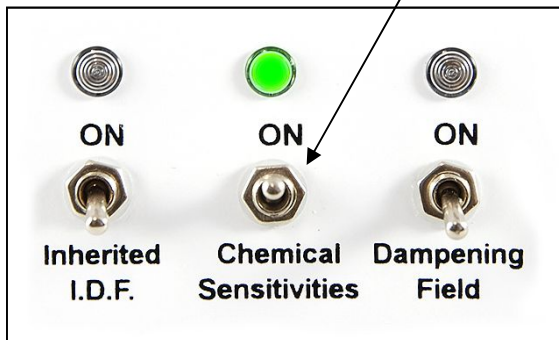

CHEMICAL SENSITIVITIES: An extreme chemical sensitivity can often be found among Subjects when they are contact with, or exposed to, such things as chemicals, vapors, cigarette smoke, smog, allergens, and environmental toxins. These Subjects may be hyper-accelerated when exposed to any of these things. The ABPA reduces the power and fine-tunes the detail of the scan.

CHEMICAL-SENSITIVITIES SWITCH: When this toggle switch is placed in the "ON" (upward) position, the ABPA lowers its own power output. It reduces the ABPA's own level of 20 Energy Units down to 2 or 3 Energy Units. It performs a more detailed scan of the Research Subject. It engages more of the built-in Safety Codes to benefit the Research Subject. The ABPA was designed so that when this toggle switch is "ON", there is a more refined scan and a more gentle transmission for those Research Subjects who have strong sensitivities to chemicals, toxins, contaminants, and allergens.

CHEMICAL TOXINS: Chemical toxins – be they airborne, in soil, water, food, or from any other source – cause stress to human, animal, and plant systems. Their source may be invisible. Their damage may be difficult to reverse. Their impact may be permanent. Pollutants may even be electronic in nature through cellular phones, wireless internet, cell towers, microwave towers, and communication satellites. Dr. Karim Ibrahim – famous bio-geometer and antiquities architect in Cairo, Egypt – refers to these pollutants as "electro-smog". The ABPA provides Countermeasures to stress caused by this "electro-smog" and other chemical contaminants, most of which are invisible to us and difficult to detect.

CLEANING THE ABPA: The ABPA is a subtle energy detection system, so everything should be cleaned before each use. The photographic Sample Well, the INPUT Well, the OUTPUT Well, and the Scan Cable should be cleaned before each use. Clean the INPUT and OUTPUT wells (especially the bottoms and sides) by using a soft facial tissue, Windex wipes, or a damp paper towel. Keep the Scan Cable, switches, lights, and body of the ABPA free of liquid drips and dust accumulation. The ABPA should always be positioned on a flat, clean surface away from moisture and liquids. Dust and dirt on the ABPA face or inside any of the three wells will not allow the ABPA to work correctly or effectively. Be certain that there is never a single hair or even a small piece of paper left in the photographic Sample Well to contaminate it. To clean the photographic Sample Well, turn the ABPA upside down and tap it gently to dislodge anything that might have fallen into the narrow slot. The white face plate should be cleaned, along with the four sides and the bottom. The ABPA can also be kept dust-free by slipping it into its original plastic bag from shipping. Just loosely close the open end of the bag, and the ABPA will run just fine. The purpose of keeping the ABPA clean at all times is to remove sample information and contamination from the previous user.




COMMON SENSE: Always seek proper medical attention first. Use other technologies, such as the ABPA, after that. Use common sense in all health matters.



CONTENTS OF YOUR ABPA PURCHASE:

- Advance Bio-Photon Analyzer – Model A2
- User Manual – what you’re reading right now!
- International Power Supply Kit** – with adaptors for overseas use
- Scan Cable – 10 feet long, black, with a green LED at one end on the tip
- Laminated “Top Ten Procedures” Sheet
- Disclaimer Information and Manufacturer’s Warranty Information
- Optional Items – additional accessories you may have ordered
- Warranty Registration Sheet – please complete the information and send it in

COPY SWITCH: The COPY toggle switch can be used to copy the energetic profile of such things as Vitamin C, Vitamin B Complex, supplements, homeopathics, and water. The Isopathic Remedy does not rapidly or readily degrade in the way a homeopathic remedy does. Place wedding ring into bottom of well. Human bodies are just an excuse for water to get up and walk around.

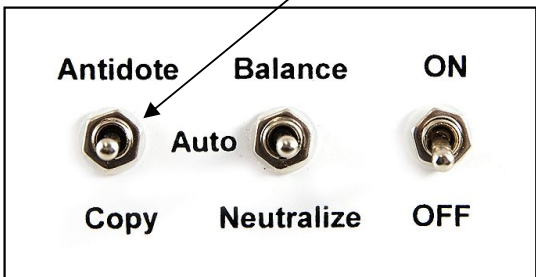

CORE GROUP OF SWITCHES: These are the group of three toggle switches located in the center of the face of the ABPA, and they include the “ON” and “OFF” switch.

COUNTERMEASURES: The Isopathic Countermeasures made by the ABPA will not degrade easily or quickly, and even then, usually only if exposed to a strong infrared or ultraviolet state. These Isopathic Countermeasures are contrasted with radionic homeopathics which will degrade more easily and quickly because radionics uses a magnetic field.



DAMPENING FIELD: When this toggle switch is placed in the “ON” (upward) position, the ABPA isolates the surrounding electrosmog environment from affecting the Research Subject. It acts as a shield to insulate the Research Subject from detrimental external energies (such as cellular phones, pagers, power grids, radio frequencies, fluorescent light fixtures, and cell towers). It creates an invisible isolation around the Subject to limit interference from outside energies. It provides an energy conduit to the Research Subject so it will find the best path with the least loss of signal, whether receiving or transmitting. It isolates the ABPA’s scanning and transmitting area to within about 24” around the Research Subject. The Dampening Field filters out electromagnetic frequencies from devices and signals which might affect your system while the ABPA is scanning. This feature makes the scan more detailed to the Subject; the scan will identify the nearby power line, but the testing scan will not be influenced by it. Most researchers leave this toggle switch “ON” 100% of the time.



DEVICE INTERFACE CABLE: The Device Interface Cable is an accessory designed to connect the ABPA with another instrument. If you wish to connect the ABPA to another instrument or outside equipment, ALWAYS check with us first at our website, www.A2SRC.com, to ask us to determine if it would be an approved device for use

"So astounding are the facts in this connection, that it would seem as though the Creator, himself had electrically designed this planet...."

-Nikola Tesla describing what is now known as Schumann Resonance (7.8Hz) in "The Transmission of Electrical Energy Without Wires As A Means Of Furthering World Peace",



with the ABPA, and if a Device Interface Cable may be needed. In certain cases, the ABPA can be connected to 1) frequency generators, 2), sweep function generators, 3) Rife machines, and 4) frequency output devices, but ALWAYS check with us first. The ABPA should NEVER be connected to 1) radionics devices, 2) bio-scanner devices, 3) bio-sweep devices, or 4) orgone energy devices. Serious damage may result from such usage and the Manufacturer's Warranty will be voided if such a connection has been made.



DISARMING: To prepare for taking a photograph to be used with the ABPA, the Subject should be "disarmed" by removing eye-glasses, hearing aids, and jewelry (some people are allergic to the metal in their own jewelry and don't know it). Photograph from the Subject's waist to a short distance above the head. Do not wear red during the time the photograph is being taken, as it confuses the photograph and makes the ABPA have to work too hard during the time it is scanning.

ENERGY UNITS: Assuming a canon between 1 Energy Unit and 20 Energy Units, a chemically-sensitive human being can usually only tolerate 2 or 3 Energy Units; a normal healthy animal usually needs about 5 or 6 Energy Units (depending on size and activity); a normal healthy human being would usually need about 7 or 8 Energy Units. The ABPA, however, has the ability to make 18 to 20 Energy Units. Wow . . .

ENVIRONMENTAL CONTAMINANTS: On a daily basis, we can all become contaminated by physical contact (such as a hairdresser handling chemicals while giving permanent waves or processing hair color) or inhalation (such as a farmer breathing nearby while herbicides are being applied to an adjoining field). Other sources of contamination can come from food, water, fumes, and air pollution.

GENERAL VITALITY and RESERVE GENERAL VITALITY: Most healthy Subjects maintain a baseline of General Vitality and a varying baseline of Reserve General Vitality. Chemically-sensitive Subjects will often have little or no General Vitality, and must rely mostly on their Reserve General Vitality for daily activity. When Subjects use the ABPA, the energetic Countermeasures will work on General Vitality and revitalize Reserve General Vitality.

HOME AND OFFICE DETOX: This is one of the "Top Ten Procedures", and you will need a 6" to 8" piece of adhesive tape, a pen, a small sealable plastic bag, and a mister bottle filled with water. To begin, inspect and clean the Wells before each use. Take a 6" to 8" piece of adhesive tape and stick it to areas and objects in the room to pick up dust and debris from floors, walls, carpet, baseboards, doors and door frames, windows and window frames, furniture, and picture frames. Fold the tape against itself, sticky side to sticky side. Label the tape with the name of the room, date, and location. Move from room to room repeating the preceding steps. Then place one room's tape sample in the INPUT well. Fill a mister bottle with water, wipe the bottle clean, and place in the OUTPUT well. Place left toggle switch to Antidote setting, and place center toggle switch to

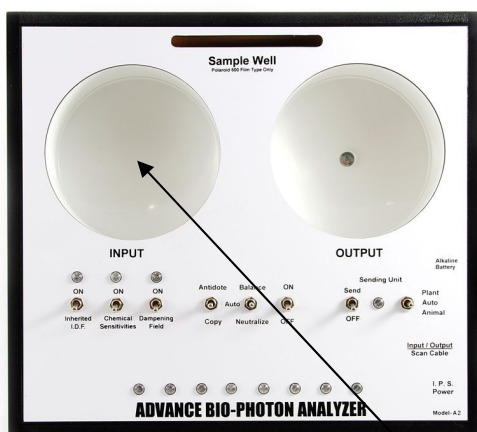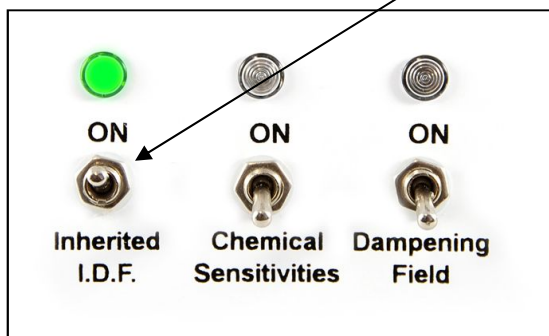

Neutralize setting. Turn the power on and run until ding-dong chime sounds. Turn power off. Reset toggle switches to Auto, Auto. Turn power on again and run until ding-dong chime sounds. Turn power off. Remove objects from INPUT well and OUTPUT well. Repeat this process until all tape samples are used. Set the mister bottle for ultra fine mist and walk through each room, gently spraying 6 to 10 pumps per room above head height. Repeat for each room from which a sample has been taken. The water mist will become inert upon reaching the floor. Repeat each week if needed.

INHERITED I.D.F. SWITCH: When this toggle switch is placed in the "ON" (upward) position, the ABPA scans the Research Subject for miasms. Miasms are genetic predispositions to illnesses or weaknesses any of us might have within our gene pool. So, for example, it scans for miasms (such as tuberculosis or syphilis) which the Research Subject might have received from blood relatives such as parents, grandparents, and great-grandparents. It scans for heavy metals (especially aluminum, arsenic, formaldehyde, lead, and nickel) that might have mutated any of the miasms, and mutated masking fragments. Miasm may be understood to be a dynamic energy which cannot be seen and is considered hostile to the life-preserving energy; every living creature on earth – bacteria, virus, etc. – has its own miasm. There is always a battle going on inside the body between the Vital Force and the Miasmatic Force. In health, the Vital Force is stronger; in disease, the Miasmatic Force is stronger. This is somewhat analogous to the Greek word "apheta" and Greek word "anareta", or life-giver and life-taker. The ABPA can scan for a miasm and provide an anti-miasmatic counter-measure. When the Inherited I.D.F. toggle switch is engaged, the ABPA works on the person who is the Subject and also includes other family direct-bloodline ancestors and descendants. In other words, it is extending itself to others within the Subject's gene pool. Researchers believe that energetic patterns may be inherited or passed down from one generation to the next. The ABPA with the Inherited I.D.F. toggle switch turned to the "ON" position recognizes the miasm, tags the miasm, makes the body aware that the miasm is within the Subject's system, then continues to work the Miasm out of the body without destabilizing the Subject's system. It scans the etherical genetic energies of the Subject to determine if a combination of genetic energies could be harmful to the Subject. With this engaged, the ABPA is recognizing a pattern that could be affecting the Subject at an etherical gene-pool level; the ABPA is trying to focus on those patterns – those miasms – when the Inherited IDF toggle switch is turned to the "ON" position. When this switch is placed in the "ON" position, the ABPA scans for etheric, genetic, cellular energy patterns of the Research Subject to determine if there are miasms, mutated miasms, or heavy metals that may be harmful. Many researchers leave this toggle switch "ON" most of the time.

INPUT WELL: The INPUT Well receives any reagent or item to be scanned. Any items used as samples for the INPUT Well should be kept clean from fingerprints and contamination.

"If you want to understand the secret behind Creation, think in terms of Energy, Frequency and Vibration".

Dr. Nikola Tesla, 1942 — inventor of AC power, radio, logic circuits, particle beam weapon theory, multiwave oscillator technology; holder of nearly 2,000 patents.

ISOPATHIC REMEDY: An Isopathic Remedy is the art and science of recovery by giving your energetic body what you need when you need it. The ABPA looks at a Subject as a frequency profile. If the ABPA finds something that is too weak, it will provide a strengthening energetic remedy. If the ABPA finds something that is too strong, it will provide an energetic remedy that will phase it out of the system. It creates a Countermeasure to create a stabilizing effect. An Isopathic Imprint is a potent, broad-spectrum, energy-charged frequency pattern technology that is capable of being received by a medium that may be based in such things as water, oil, alcohol (primarily vodka), or glycerin. By way of contrast, a homeopathic is magnetically-encoded; an isopathic is photon-charged, or light-encoded. An analogy might be a homeopathic which would be similar to a computer floppy disk which is encoded magnetically; conversely, an isopathic would be similar to a CD-ROM or DVD which is encoded optically, using a laser.

KINESIOLOGY IMPRINTING: Inspect and clean wells before each use. Place one hand into the INPUT Well, and use the opposite hand to touch a point on the body, and hold that position. Place the Target Object into the OUTPUT Well. Place left toggle switch to Antidote setting, and place center toggle switch to Neutralize setting. Turn the power on and run until ding-dong chime sounds. Turn power off. Reset toggle switches to Auto, Auto. Turn power on again and run until ding-dong chime sounds. Turn power off. Remove hand from INPUT Well and target object from OUTPUT Well.

MAINTAINING THE ABPA: The ABPA would probably appreciate your keeping it clean, look on it kindly, treat it nicely, and provide a little niche that it can call its own. If you feel Warranty service may be required, or you would like to know if there are ABPA software and hardware updates available, or you would just like to have your ABPA checked out every year or two, please contact the ABPA Service and Repair Center at its website, www.A2SRC.com.

MIASMS: Miasms are genetic predispositions to illnesses or weaknesses any of us might have within our gene pool. So, for example, the ABPA scans for miasms (such as tuberculosis or syphilis) which the Research Subject might have received from blood relatives such as parents, grandparents, and great-grandparents. It scans for heavy metals (especially aluminum, arsenic, formaldehyde, lead, and nickel) that might have mutated any of the miasms, and mutated masking fragments. When the **"Inherited I.D.F."** toggle switch is placed in the **"ON"** position, the ABPA scans for etheric, genetic, cellular energy patterns of the Research Subject to determine if there are miasms, mutated miasms, or heavy metals that may be harmful.


MINERALLY-SOUND: All Research Subjects should be minerally-sound. Minerals activate vitamins. All of us should take enough trace minerals to keep healthy, as often even what we think is a sufficient intake of food and liquids can be lacking to provide adequate nutrition and minerals. The ABPA will prove to be less helpful if the Research Subject is minerally-weak, because the ABPA looks at the Subject on a mineral basis. During illness, the minerals in the body





are usually neither strong nor distributed evenly. The ABPA needs to have enough information to make a positive decision for the best course of Countermeasures for the Research Subject, and being minerally-sound is an important part of that.


MINERALS: We are mostly made of water and minerals. Animal and human bodies need to be well-mineralized to allow the ABPA to work correctly and accept the ABPA Countermeasures. If you are mineral-deficient, the ABPA will not be able to recognize as much of your energetic profile in the Subject photograph as if the Subject were well-mineralized. It is easy and inexpensive to take one or more packets of something like "Emergen-C" (available at most big box stores such as Wal-Mart, Walgreen's, and pharmacies) or other all-trace minerals every day. With not enough minerals, the ABPA will see the Research Subject as transparent. With enough minerals, the ABPA will see the Research Subject as opaque and can determine a healthful course of action.

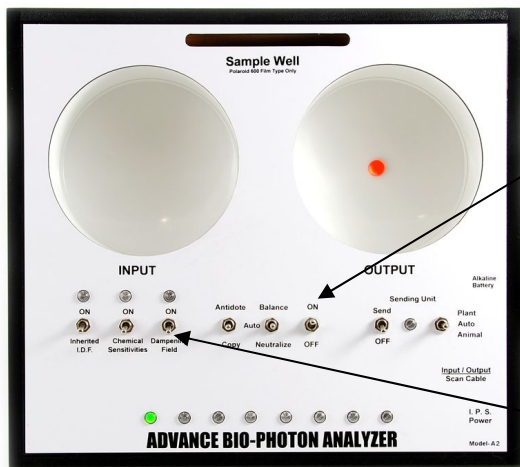

ON – OFF SWITCH: This toggle switch turns the unit on and off. This toggle switch set in the "ON" position turns the unit on and prepares it to accept any other settings you choose. This toggle switch set in the "OFF" position turns the unit off and all setting selections are disengaged.

OPTION SWITCHES: These are the group of three toggle switches designated "Inherited I.D.F.", "Chemical Sensitivities", and "Dampening Field".

OUTPUT WELL: The red light in the bottom of this well is known as the "Imprinter". (Remember to never look directly at ANY laser light, including this one.) It is an optically-charged device that is making the Countermeasure and it is sending it vertically from the bottom of the OUTPUT well.

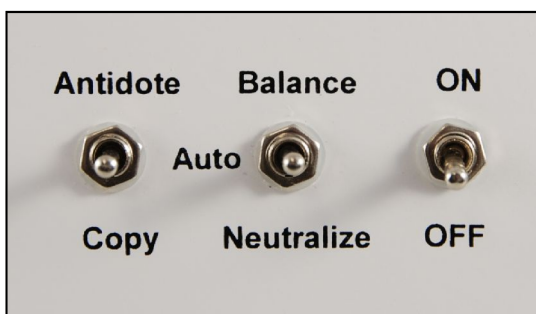

PHOTOGRAPH A PERSON: If the Research Subject is a person, it is recommended that the person be photographed from the waist up, wearing a neutral top (never the color red while taking the photograph), with as much bare skin showing as possible, holding both hands up at about ear level, and fingers extended. It is easier to work with a photograph than a physical biological sample. Handle the photograph on the wide strip only. Do not touch the front, back, or sides, as the oils from your fingers will degrade a photograph of someone other than yourself. Have only one Subject appear in the photograph. The photograph can be taken either on the square or the diagonal.

PHOTOGRAPH AN ANIMAL: If the Research Subject is an animal or pet, such as a dog, cat, bird, horse, cow, goat, sheep, or other critter, it is recommended that the animal be photographed once to include its whole body, and then a second time as a close-up if there is a particular area of concern. And, as with a human being as a Research Subject, the background should be neutral or light-colored (never the color red while taking the photograph). No other living beings or electronic devices should appear in the photograph.

PHOTOGRAPH ARCHIVING: There can be great research value in taking a series of photographs and archiving them. Practitioners are advised to keep a patient file of photographs which can be placed in a clean, sealed, plastic bag with information noted (to include such things as patient's name and the dates and locations of the photographic record series) and stored as a patient reference. Similar archiving should be done by veterinarians who wish to keep a photographic record series of pets and animals that have used the ABPA.

PHOTOGRAPHIC BACKGROUND: In nearly all cases, the photograph should contain only one Research Subject. The background should be a neutral or light-colored. There should be no other distractions in the background, such as art, plants, pets, lamps, electrical outlets, light switches, power cords, door frames, window frames, television sets, or other electronics. The color red should never be in the photograph – either as clothing, an accessory, or a part of the background. There should be no other living beings in the photograph. Do not take a photograph of a group of people with the idea of using the photograph of only one person from the group.

PHOTOGRAPH HANDLING: Place the photograph of the Subject into the Sample Well, taking caution to not touch the photograph with your fingers (hold the photograph by the wide edge strip to avoid getting oil from your fingers on the photograph's Subject area). The wide edge strip is also a good area to write the name of the Subject along with the date and location that the photograph was taken. Put the photograph in upside down, facing either toward the front or back, by holding the wide edge strip at the top. Be careful to keep the photograph clean and untouched by fingerprints. Multiple photographs of the same Subject, all taken with Polaroid 600 Film, can be used simultaneously in the photographic Sample Well.

PHOTOGRAPH OTHER RESEARCH SUBJECTS: If the Research Subject is a plant, tree, garden, yard, swimming pool, or field, it is recommended that the plant or area be photographed to include as much of the area of interest as possible. If the Research Subject is a herd or a flock, it is recommended that the entire group be included in one photograph. For example, multiple photographs of a room or a building or other Subjects can be taken and several of them could be grouped together and placed in the Sample Well at the same time. (Always be careful to put all the photographs in by holding their wide edge strips.) Another experimental use might involve taking a Polaroid 600 Film photograph of a property you wish to sell. Put the Subject photograph in the Sample Well, and engage the Sending Unit for continuous broadcasting. (Maybe you'll be able to get even a crummy property to sell!)

PHOTOGRAPH UPDATES: Most researchers update their photographs from time to time, as they recognize conditions changing within their Research Subjects. This can be as often as daily, or as infrequently as several months, but never longer than 6 months. Also, if there are mishaps, traumas, or accidents, new photographs



should be taken immediately. Another advantage of updating photographs is that there is, by comparison, a method of subjective measurement to observe the progress of the Research Subject's physical appearance while using the ABPA.



PROCESS INDICATOR LEDs: There are eight brushed stainless steel toggle switches placed across the face of the unit from left to right. They indicate that a process is occurring, as they appear with green lights sequentially from left to right for a period of 40 seconds. Never turn power off during the 40 seconds while the green lights are cycling.

SAFETY CODES IN THE ABPA: The ABPA has been designed to include built-in Safety Codes. These Safety Codes are unique only to the ABPA. Although Safety Codes look as small as a single line on a screen, this feature is actually one of the most important and most exceptional features of the ABPA. Safety Codes actually prevent the subject from being harmed. If the Subject is not in the best of health, or the Subject is attempting to recover or regain health, the Safety Codes will prevent the Subject from accepting the potencies if the ABPA determines that they are too high, or too strong. The ABPA Safety Codes will allow the Subject to refuse a too-excessive potency. The ABPA adjusts the Countermeasures to always allow the Research Subject to stay in a state of balance. It is the only instrument in the world that has Safety Codes built into it.

SAMPLE COLLECTING: We recommend the use of a photograph (using Polaroid 600 film) of the subject (in front of a neutral wall with no background distractions), small fingernail and toenail clippings, horse saliva on a piece of cotton, pet hair, adhesive tape (which has been used to collect environmental samples from the home such as dust and dirt from walls, furniture, carpets, heating and air vents). To use hair or fur as a sample from a pet, carefully cut a sample of hair or fur and seal it in a small plastic bag, and place it in the "Input" well. To collect outdoor contaminants, a blotter agent, such as a coffee filter, can be tacked to a post or tree and left there to collect for a few days, or for a few weeks. Then the contaminated coffee filter should be placed in a sealed plastic bag and labeled to identify the area, date, and location. Biological Samples degrade more quickly than Photographic Samples. You can also use mercury from your teeth, or amalgam fillings, as samples, along with a photograph. (This concept has been around since 1989.) Samples such as blood, nasal mucous, and pus are considered biohazards and are not recommended. However, they can be used in a pinch. Most of the time, more appealing options are available.

SAMPLE OBJECT: A Sample Object is an object which would be placed in the INPUT Well or in the photographic Sample Well, ready to be energetically scanned.

SAMPLE WELL: The photographic "SAMPLE Well" is located at the top of the face of the ABPA and is about 3-1/2" square. It has been sized to hold one or more photographs, or some other flat sample

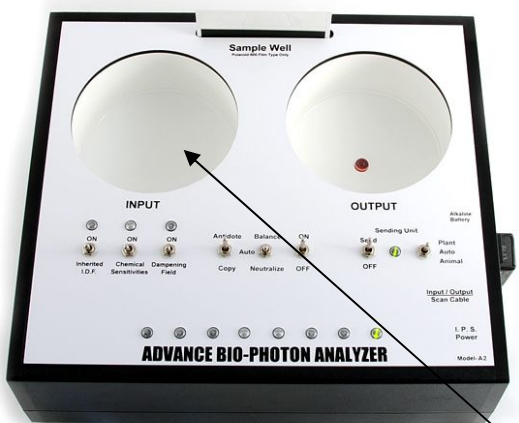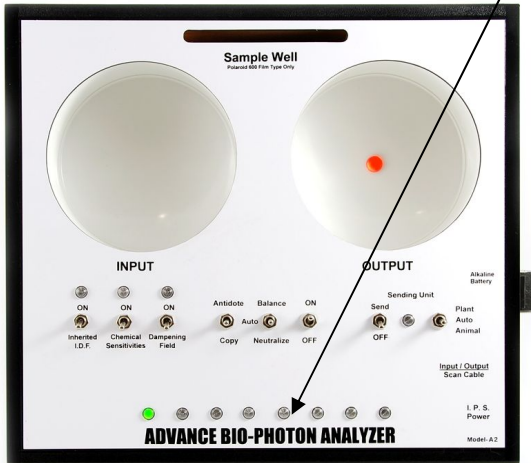





which can be placed in a plastic bag and inserted like a photograph. Be careful using this well, as it cannot be easily cleaned if it becomes contaminated. Also keep in mind that photographs placed in the Sample Well can be used in conjunction with most biological samples (such as hair, saliva, skin, fingernail clippings, toenail clippings). Less desirable samples (such as blood, nasal mucous, and pus) are biohazards, and should only be used in a pinch. Those samples, if they must be used, should be placed in a new, clean, sealed plastic bag and placed in the INPUT well. Any of these biological samples can be used simultaneously with photographs placed in the photographic SAMPLE Well.

SAMPLES TO AVOID: The ABPA needs an active RNA/DNA bio-energetic property to work from. It needs real energy to work from. Do not use Polaroid spectrum film. Do not use 35 mm film. Do not use a hand-written note or a hand-written signature. Samples such as blood, nasal mucous, and pus are considered biohazards and are not recommended. However, they can be used in a pinch. Most of the time, more appealing options are available.

SCAN CABLE: The Scan Cable is 10 feet long and has a mini-phono plug on one end and a green light on the tip of the other end. It should be plugged into the receptacle on the side of the ABPA. The Scan Cable broadcasts emissions about 12 inches in all directions along its length. It can be wrapped loosely around such things as tennis elbows and sore muscles (usually caused by uric acid accumulation, inflammation, strain, and overuse).

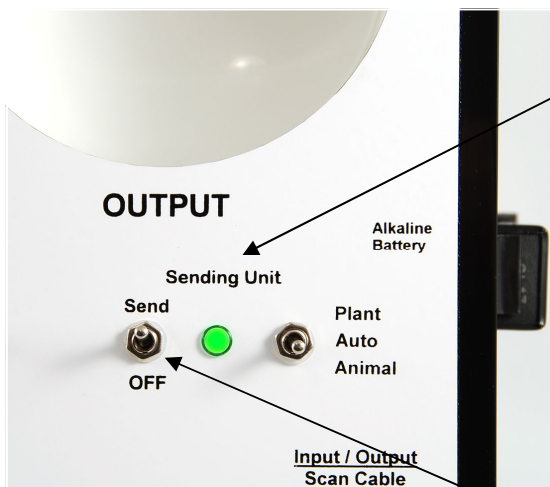

SENDING UNIT: The Sending Unit is a built-in transmitter, capable of broadcasting energetic Countermeasures to Targets, regardless of their location. The US Navy has used a "Rainbow" antenna located in the Michigan Peninsula which was designed to transmit low frequencies through the earth for communications purposes. The ABPA utilizes a very low frequency transmitter in the Sending Unit which transmits at approximately 4 Hz to 26 Hz, depending on the setting of the toggle switch labeled "**PLANT-AUTO-ANIMAL**". When the Sending Unit is on, the ABPA performs an on-going sensitive fine-tuning. It will perform a continuous, alternating 40-second scan, then a 40-second transmission, then a 40-second scan, etc. This is especially helpful for a chemically-sensitive Subject who needs constant fine-tuning to stabilize. No ding-dong chimes will sound when the Sending Unit is operating.

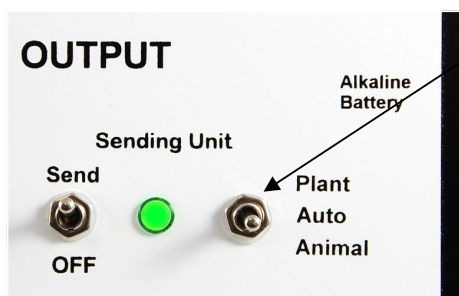

SEND – OFF SWITCH: When the toggle switch is placed in the "**SEND**" (upward) position, the Subject will be stabilized, and brought to a balance point. When the **PLANT-AUTO-ANIMAL** toggle switch is set, it specifies different octaves of energy. When the toggle switch is set to **PLANT** it is at low-level cellular of the body, and is transmitting at about 13 Hz. When the toggle switch is set to **AUTO** it is equivalent to the mineral kingdom, and is transmitting at about 26 Hz. When the toggle switch is set to **ANIMAL** it is complex, and equivalent to the high-level nervous system of the body, transmitting at about 4 Hz. The Schumann Frequency varies, but is about 7.83 Hz. If you are uncertain, set the toggle switch to **AUTO**.




STRESS: Stress of any kind – cellular (which causes aging), emotional, energetic, mental, neurological, physical, or psychological – is easy to come by, and something all of us have way, way too much of. You cannot “cure” stress. You cannot “heal” stress. However, you can learn to diminish stress, and recover from it. The ABPA is a stress-management-system instrument.

TARGET OBJECT: The Target Object is vial, bottle of water, or other object that is placed in the OUTPUT Well and is ready to receive the energetic Isopathic Remedy or Isopathic Countermeasure.

WARRANTY EXCLUSION: Warranty Exclusion may occur if the ABPA has been breached or tampered with. The ABPA (A2 and AM3) System uses tamper-proof screws and sets to protect the Wave Guide in the unit. The Wave Guide is a precision-tuned alignment device that is required for the Safety Codes to function. Without this Wave Guide, the Safety Codes may not function correctly. If the enclosure is opened or breached, the Wave Guide will be altered from the original factory setting. This will cause the unit to render a neutral safety function within the unit and corrupt the software so as to prevent downloading from occurring. If the A2 Service and Repair Center finds such tampering to alter, modify, or re-create the device, the Manufacturer’s Warranty will be voided. The A2 Service and Repair Center will not repair or replace the unit.

WELLS: There are three Sample Wells on the face of the ABPA, and all are tied together on the same scanning circuit. There is a scanning capability feature in the bottom half of all three wells, so you can provide as many samples as you wish. Therefore, as much as possible, your photograph samples and your biological samples should be in the bottom half of each well. The photograph Sample Well is square, about 3.5” in length. The INPUT Well and the OUTPUT Well are circular, about 4.25” in diameter. They have been sized to receive a one-quart jar, or a good-sized bottle of water.

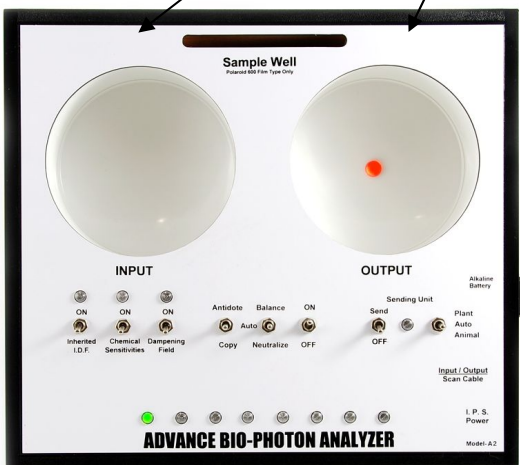

Non-locality in quantum theory is discussed in terms of the global form of the wave function, and as subtle set of necessary and sufficient conditions on the 2-matrix or reduced density matrix. In addition to manifesting itself through the well known Bell's inequalities non-locality also appears as a macroscopic coherence length in condensed and coherent systems. By examining the structure of the 2-matrix, a connection between these two forms of non-locality is made. It is suggested that subtle enfolded orders and non-local forms may have a wider implication and be relevant for a variety of living systems.

--from Bell's Theorem

AM3 Quick Start Guide



Congratulations upon your purchase of the AM3! These guidelines should make your AM3 easy to use, even for the first time.

The theory of the AM3 is the creation of an oscillating magnetic field which sets up a pattern of resonance which causes the cells of the body to begin to re-synchronize in a coherent pattern. It is analogous to the chaos of a marching band whose members are all out of step, and the band director blows the whistle to put them into uniform step. Each cell's energy starts to re-synchronize with all other cells and all of the body systems start working together harmoniously.

Special warnings before using:

1. Always keep the Magnetic Pad clean. The Magnetic Pad should never be washed or dry cleaned; only modest cleaning can be done with a lint roller, or spot-cleaning using a soft, damp cloth. Never immerse in water.
2. Always keep the Substance Well clean (using a tissue lightly sprayed with window cleaner).
3. Always keep the Solution Well clean (using a tissue lightly sprayed with window cleaner).
4. The AM3 must be powered using the International Power Adaptor. The AM3 must never be powered by using a 9-volt battery.
5. For maximum benefit, the research subject should be adequately hydrated and mineralized.
6. Never plug the LED Scan Cable into the "Pad Output" jack.
7. Never plug the Magnetic Pad into the "Scan Cable" output on the right side of the Control Box.

An International Power Supply (IPS) is provided with the AM3. Only this IPS is to be used both in the U.S. and overseas. The IPS kit comes with a variety of tip adaptors which enable use in most countries overseas. Do not use the AM3 or the IPS with any other type of voltage converters or inverters. This may damage the AM3 and will void the warranty.

VERY IMPORTANT: Never turn on the "On/AM3" switch on the top of the Control Box and press the Green "Start" button on the left side panel at the same time. This could seriously damage the electronic components.


The AM3 System Complete contains the following components:

1. AM3 Control Box (master unit, with three independent computer boards inside)
2. Magnetic Pad (contains both magnets and electronics) and Attachment Wire
3. International Power Supply (IPS)
4. Instruction Manual
5. Quick Start Guide
6. Warranty Information

Setting up the AM3 for its first use:

Your AM3 is designed so that you can set it up quickly and start using it right away. The following information will take you through the set-up process, including these tasks:

1. Plugging in the AM3 International Power Supply (IPS)
2. Connecting the two cables
3. Setting switches and functions
4. Turning on the AM3 Control Box

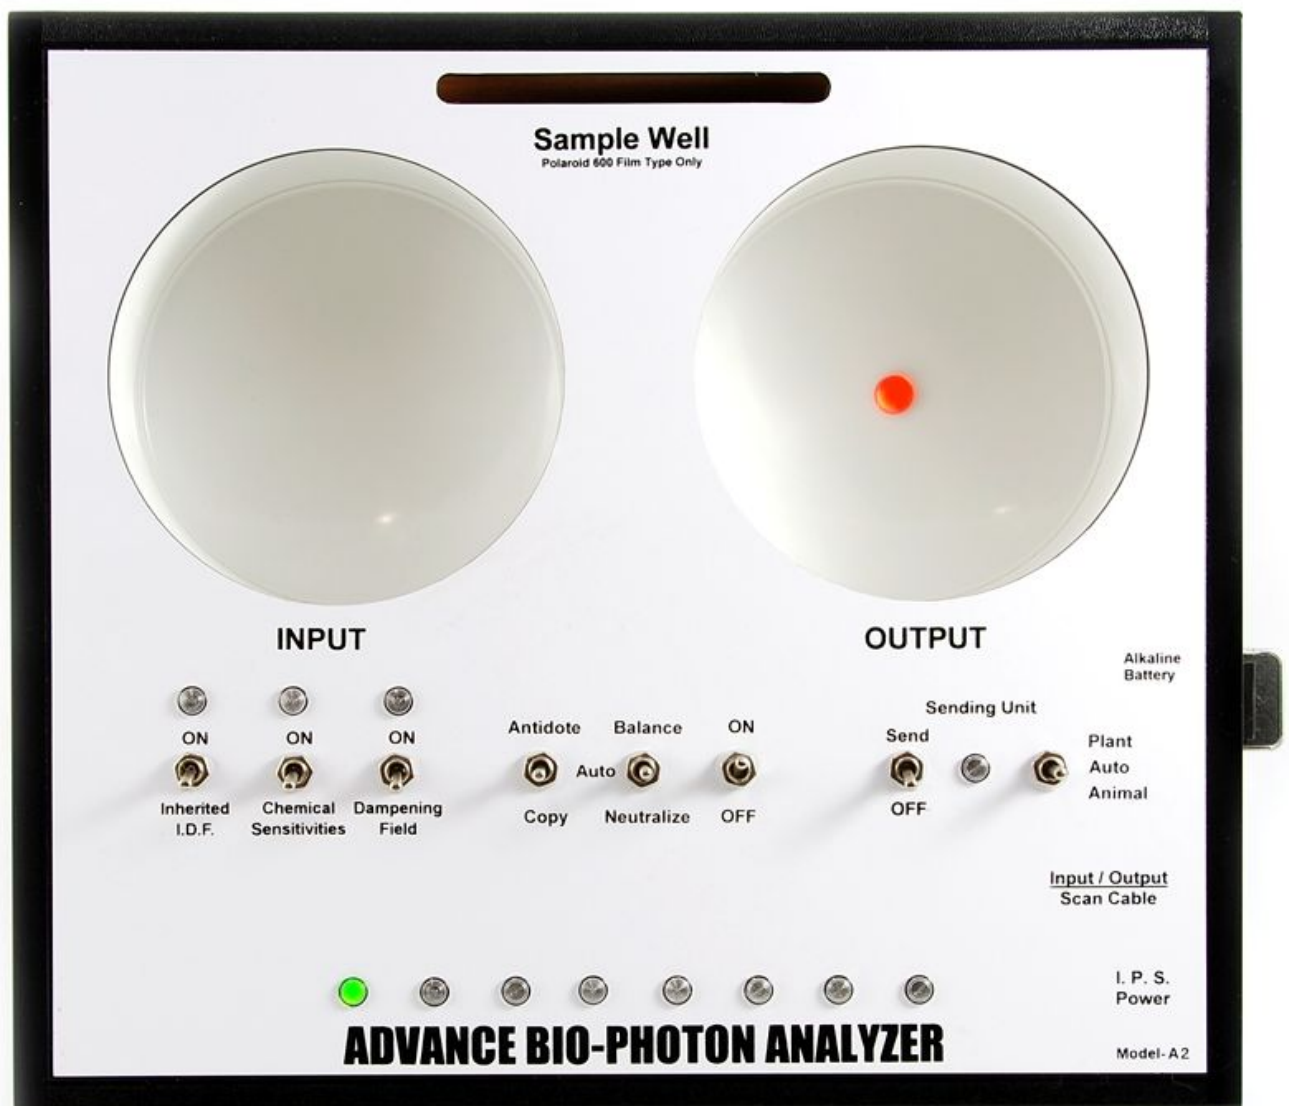

Step 1: Place the AM3 Control Box on a large, solid surface near a wall outlet. Plug the International Power Supply (IPS) into your wall outlet. Plug the small barrel connector of the International Power Supply (IPS) into the receptacle marked “Power” on the right side of the AM3 Control Box.

Step 2: Place the Magnetic Pad on a firm, large surface (such as a bed or massage table). Cover the Magnetic Pad with a blanket or sheet (to keep it clean). The Pad should be placed with the smooth side (negative polarity) facing up and the seamed side (positive polarity) facing down.

The Magnetic Pad is comprised of a series of magnets placed in a specific geometrical arrangement. The magnets are polarized so that the negative polarity radiates upward through the smooth side and the positive polarity radiates downward through the seamed side.

Step 3: Plug the Magnetic Pad’s Attachment Wire into the receptacle marked “Pad Output” on the left side of the AM3 Control Box.

Step 4: Switch the “On/AM3” switch on the top of the Control Box down to “AM3”.

Step 5: Switch up the “Power” switch on the left side of the Control Box to “AM3”. This is the normal position that the switch should be in when the ANNA sequences are being run. The only time the “Power” switch on the left side of the Control Box would be positioned in the down “Matrix 3” position would be if you wanted to apply the 7.83 Hertz or 12.00 Hertz frequencies to a subject without running the ANNA sequence.

Do not press the “Start” button if the “Power” switch is in the down “Matrix 3” position. When the “Power” switch is in the down or “Matrix 3” position, the Magnetic Pad continuously radiates the chosen frequency.

Step 6: Place the switch marked “Frequency” on the left side of the Control Box in the up position marked “7.83 Hertz”.

The Schumann Earth Resonance is generally accepted to be 7.83 Hertz. This setting has been found to be the most beneficial when used in the Earth’s northern hemisphere.

The Rain Forest Resonance is generally accepted to be 12.00 Hertz. This setting has been found to be the most beneficial when used in the Earth’s southern hemisphere.

Step 7: Place the switch marked “Positive/Negative” on the left side of the Control Box in the down position (“Negative”). This is the optimal setting for most applications.

The “Positive/Negative” switch controls the polarity of the electro-magnetic grid layer within the Magnetic Pad, but does not refer to the polarity of the magnets themselves.

If your goal is elimination (such as eliminating allergies), place the switch in the “Negative” position. If your goal is to promote or stimulate (such as promoting well-being), then place the switch in the “Positive” position.

Remember that the “Positive” and “Negative” refers to the electro-magnetic polarity of the Magnetic Pad, and not the magnets themselves.

Step 8: On the top of the Control Box, place the “Inherited I.D.F.” switch into the down (or off) posi-

tion. Place the “Chemical Sensitivities” switch into the down (or off) position. Place the “Dampening Field” switch into the down (or off) position.

Step 9: On the top of the Control Box, place the “Antidote/Clone” switch into the center position marked “Auto”. Place the “Balance/Neutralize” switch into the center position marked “Auto”. Confirm that the “On/AM3” switch is in the down or “AM3” position.

Step 10: On the top of the Control Box marked “Sending Unit”, place the “Send/Off” switch into the “Off” or down position. Place the “Plant/Auto/Animal” switch into the center “Auto” position.

It is not necessary to place a photograph of the subject into the “Photograph Well”. Nor is it necessary to place any remedies into the “Substance Well INPUT” or “Solution Well OUTPUT”. The Magnetic Pad itself acts as an independent unit and therefore the subject can rest on the Magnetic Pad only. No photograph or remedy is necessary when a subject is using the Magnetic Pad.

The Magnetic Pad can be draped over the back of a horse, a large dog, or other animal, keeping in mind that the smooth side of the Magnetic Pad is away from the animal, and the seamed side of the Pad is toward the animal.

Step 11: Set the rotary “Timer” knob (referred to as the ANNA knob and pronounced like a girl's name, Anna) to the desired number of ANNA procedures. ANNA stands for Antidote-Neutralize-Auto-Auto. It takes approximately 90 seconds of time to complete one ANNA sequence.



There are five settings for the rotary “Timer” knob:

1. “Cont” – continuous, meaning the instrument will run through ANNA continuously, without stopping (24/7/365)
2. “ANNA” – meaning the instrument will run through only one ANNA sequence, and stop
3. “5” – meaning the instrument will run through 5 ANNA sequences, and stop
4. “10” – meaning the instrument will run through 10 ANNA sequences, and stop
5. “15” – meaning the instrument will run through 15 ANNA sequences, and stop

The preferred setting is “5”, meaning that most researchers have found that five ANNA sequences produce the most beneficial results in research subjects. This is what most practitioners would use.

If there is a more stubborn issue, such as a very stubborn allergy elimination, then the rotary “Timer” knob should be set to either “10” or “15” ANNA sequences.

Step 12: On the left side of the Control Box, press the green “Start” button. This will begin running the selected program.

There are four indicator lights on the left side of the Control Box located above the “Start” button, which indicate the ANNA sequence is currently running. The two Antidote-Neutralize LED lights will illuminate during the first half of the ANNA sequence, after which it automatically clears the buffer memory. The two Auto LED lights will illuminate during the second half of the ANNA sequence. The instrument will chime either once or twice at the completion of the selected program.

Most practitioners have found that once the settings and switches have been set on the AM3 Control Box, it is best to just leave them at those settings for future use. As a general rule, the settings remain, and only the green “Start” button is pressed.

Very Important Special Notes:

On the left side panel of the Control Box located above the “Pad Output” jack, there are two additional jacks labeled “Remote Start” and “Remote Input”, which are not used. These two additional jacks are simply made available for future expansion capability and there are currently no accessories that plug into these jacks at this time.

Once the “Start” button has been pressed and the instrument is operating, never interrupt the sequence. Once it is in motion, do not make any adjustments or changes to the sequence. (If you do, you may damage the instrument and the repair may be costly.)

Also, while the process is going on, safety codes are being activated; if you interrupt the sequence, certain essential safety codes may be omitted. You could corrupt and damage any Isopathic imprint or pattern which is being created.

VERY IMPORTANT: Never turn on the “On/AM3” switch on the top of the Control Box and press the Green “Start” button on the left side panel at the same time. This could seriously damage the electronic components.

While using the AM3 portion of the Control Box, the user has the choice to select any of three advanced functions switches (which are the “Inherited I.D.F”, the “Chemical Sensitivities”, and the “Dampening Field”), and the option of using either the “Sending” unit switch or the “Plant/Auto/Animal” switch. The “Antidote/Clone” switch, and the “Balance/Neutralize” switch must always remain in the center “Auto” position while using the AM3 portion of the Control Box.

For more information.
Please go to the
A2SRC.COM
website

Innovative Concepts

“Always Moving Forward”

Warning: As of January 2009 Innovative Concepts has changed the Pad to the Mat. We are getting very positive feedback on the new Mat, both performance and durability. This Mat contains VERY Powerful rare earth magnets. **DO NOT** allow anyone to lay or use the mat while they have credit cards or any magnetic sensitive cards or devices on them also including pace makers.

“I have personally lost 2 cards myself, Alan Back, N.D.”

When you get your new mat, un-roll it and allow the wrinkles to relax. The mat will become stressed while being confined in a small box. The wrinkles will disappear over the next 24 hours or so, just be patient and enjoy the new mat.

To use the New Mat, install on table or bed like shown below.



**Connect to Pad
Output on AM3**

10' Cable is located under Mat

More information will be posted on the A2SRC.Com website soon.

Thank you,
Alan Back, N.D.

Digital Media Interface Data Sheet

Digital Media Interface

The newest product from Innovative Concepts (IC) is the Digital Media Interface (DMI). A sad day has come when the Polaroid company has stopped making Polaroid 600 film that many of us has come to depend on for our work and results. Over the last 3 years IC has been working secretly on a new cutting edge product to replace the Polaroid 600 film. After many prototypes we finally arrived at the new DMI. The DMI is able to be used in all Advance Bio-Photon Analyzers models A1, A2 & AM3 system along with all Radi-omics type units that previous received the P600 film and the SE5 as well. By simply connecting the computer USB printer cable to the DMI you can move a single photo onto the DMI and then placing the DMI into the receiver well as shown below you can use the unit just like before with just as good results. If your using a remote software program like "www.mesh.com" "logmein" or "go to my pc" you can move digital photograph in and out of the unit from any where in the world easier and simpler then ever before.



Features


- The only unit on the market that uses phase conjugation software.
- Over comes the geo-synchronous stationary obstacles that are plagued by just using the stand alone USB thumb drive with digital photographs.
- The DMI can actively track a subject like the P600 film has while keeping a bio-feed back loop. Unlike the USB drive which is a mono path only. Simply said "Stand on the "X" and don't EVER move. I'm not tracking you"
- With remote software you can remotely move digital photographs on and off the DMI while not even being in the same zip code or country.
- The DMI must be powered all the time either by the USB cable or by the power supply that comes with it. **IPS -International Power Supply (optional)**
- The DMI can receive factory updates for the all ABPA models only.
- The DMI has a "POST" (power on system test) to tell if it is working correctly or not. The DMI will routinely reset it self to clear the buffer. The DMI can runs for months without the buffer getting full and crashing.

Specifications

Weight: 6 ounces.
 Battery Power: 9 Volts Alkaline (optional)
 A/C Power: 9VDC @ 300 Ma a/c wall plug
IPS -International Power Supply (optional)
 Plastic Type: ABS Plastic
 Warranty: 3 Year Limited
 Drop resistance: 3 feet
 Software Knowledge: None needed
 Internal software: Proprietary Sealed
 Airport X-ray scans: Yes, Safe
 Digital photos size must be 1700kb or larger
 Digital photos must be 5 megapixel or higher
 Red coloring is no long an issue with photos
 Photo type: JPG or BMP are the only types
 USB printer cable (not included)
 Digitals photos emailed over the internet are ok

Can not use photographs posted on internet
Can not cut, paste or alter original photo.
Emailed over the internet is OK to use.

For more information contact your local distributor or visit A2SRC.com

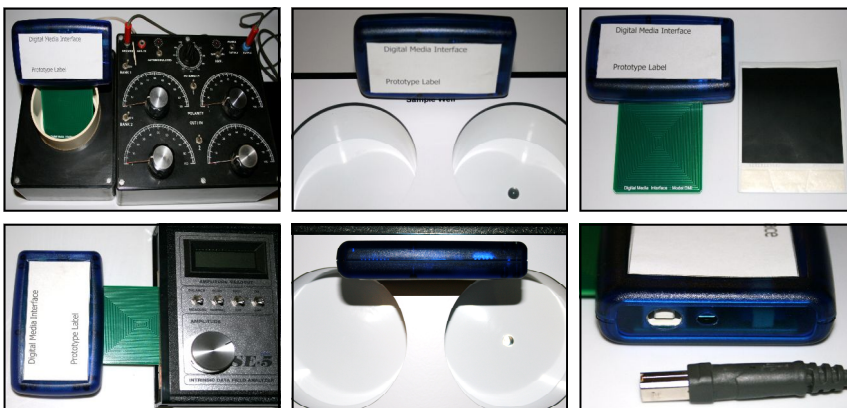

Digital Media Interface

How to use Instructions:

First I would like to be very clear about this unit. The Digital Media Interface or DMI has been designed with a series of **LAWS** that must be followed for the unit to work correctly these (5) laws are as follows.

- Law 1 - The photograph must be taken with a 5 Megapixel or higher in resolution camera. The reason for this is I don't want any one think they can take a photograph off of a website from the internet and just use it.
- Law 2 – Each photograph size must be 1700kb (1.7mb) or larger. It can be as lager as 50,000kb or (500mb) per photo graph. Again this is the 2 law of safety so no one can take a random photograph off a website site and just use it.
- Law 3 - When using the DMI you can **ONLY** have one person loaded onto the DMI drive at a time. If you place more then 1 photograph you will have co-mingled energy and this will confuse the DMI targeting software.
NO altering or cut and paste, all photos must be original and untouched.
- Law 4 – The unit must have power connected and be running for the DMI to work correctly. The DMI was designed to work as an active system not a passive system. **Do not use DC or USB together.**
- Law 5 – There are 2 file folder located on the DMI drive. (1) The folder titled "Subject" is the folder that the software will scan from. This is the only place on the drive a photograph can be placed and used. (2) The second folder titled "Updates" is for future software updates for the Advanced Bio-Photon Analyzer model A1, A2 and AM3 system **ONLY!** Once you register your DMI you will be email the updates. This means you will not need to send unit A1, A2 or AM3 unit back in for software updates they will be updated on the DMI drive. If you see the need to move the DMI unit to another ABPA unit the updates will work on that unit as will. At this time it is limited to just these models however, we may see the need to expand it in the future, if so we can.

How to connect your unit to the computer:

For simple practices will use the Advanced Bio-Photon Analyzer model A2 for our example.

- Step 1 - Unpack the Digital Media Interface (DMI) from the shipping box you will have the following items.
The DMI unit and the paperwork for warranty and instructions.
The power supply (this is not an IPS supply) the IPS can be purchase separately for oversee order or uses.
For oversee use DO NOT use a convertor the warranty will not cover it only use an IPS.
- Step 2 - Connect the USB printer cable to the DMI and computer. Will work the same for MAC or PC
- Step 3 - Your computer should find the DMI drive and be labeled as example "**E: DMI 1000**"
- Step 4 - Move your digital photograph (see laws 1, 2 & 3) into the file folder marked "Subject"
- Step 5 - If you choose to power the DMI from the USB cable simple place the DMI into the "Sample Well"
- Step 6 - If you do not need to have the computer connected, then use the power supply only **not both.**
- Step 7 - Place the DMI into the sample well or reference well or slot (On SE-5 or Radionics unit place where you would normally place the Polaroid 600 film (P600)
- Step 8 - Use your unit like you would normally would.

Remote software:

One of the free programs I used to test the DMI was www.mesh.com or "log me in". With the mesh service you will need to have a free "hotmail" or "live" email account. There are many cool features to mesh program however once you have Live Mesh Beta setup on between 2 computers you can remotely move photographs from the computer onto the DMI from a different location. In the short near future I will make a short video and post it to the A2SRC.com website so just be patient I'm working as fast as I can.

P.O.S.T. - Scanning and tracking Indicators:

The DMI has a Power On System Test or P.O.S.T. for short, it will start every time you connect power to the DMI. The DMI has 3 Light Emitting Diodes (LED's). The LEDs are used to verify the performances and diagnostic of the DMI as it works. The DMI will power up and run an internal series of checks shown below, this sequence will run 1,2,3 and then the #2 will blink (X) number of times to indicate the version of software loaded we are currently using Version 3 so it will blink 3 times. Then it will sequence 3,2,1 after 1 all indicators should go out for 1 to 2 seconds. The DMI is loading the final software to run the unit. For normal operation the #2 and #3 LED will blink the #1 LED will stay on without blinking. At this time the DMI is functioning correctly and properly. "**POST 1,2,3 2,2,2 3,2,1**"

Thank You,
Dr Alan Back

 3 Scanning / Receiving

 2 Transmitting

 1 Power

A2/AM3

WARRANTY AND SERVICE INFORMATION

THREE-YEAR LIMITED WARRANTY

The following warranty policy applies only to the original customer of this product and is not transferable. Evidence of original purchase is required for warranty service. (Include the sales receipt, packing slip, or warranty form mail in.)

Your warranty will expire if you do nothing. The Owner has 30 days to complete the Warranty form section below and return it to the address below for it to be valid. All Serial numbers and dates of creation are recorded in the central computer from the manufacturer.

Elements of Warranty

Innovative Concepts warrants this product to be free from defects in materials and workmanship for a period of three years from the date of purchase, to the original customer, under intended normal use, subject only to the limitations and exclusions set below.

Warranty Limitations and Duration

- A) This warranty to the original consumer shall terminate and be of no further effect 36 months (3-years) after the date of the original purchase. This warranty is invalid if this product is: Used for private or commercial rental purposes. Extended warranty can be purchased after the 3 year factory warranty expires
- B) Damaged, carelessly or improperly maintained, misused, abused, dropped or is not operated in accordance with the operating instructions as explained in the user manual.
- C) Serviced or repaired by persons other than an Authorized ABPA Repair and Service Center.
- D) If the user or person's modified, altered or tampered with products of Innovative Concepts. Innovative Concepts will classify the product as "DESTROYED" and will not refund the cost of the product to the distributor. These "DESTROYED" items are not subject to be refundable by the Innovative Concepts, Distributor or product manufacture.
- E) Damaged due to natural disaster including but not limited to Water (rain, flooding), Wind, Lightning or Power surges.
- F) Used in conjunction with equipment or connected to, parts or as part of any system not authorized or manufactured by the Innovative Concepts.

Statement of Remedy

In the event the product does not conform to this warranty at any time while in effect, Innovative Concepts at their option will repair and correct without charge for parts or service, any defects which are the direct result of faulty materials or problems with the normal operation due to the manufacturing process and/or workmanship. **This limited warranty set forth is the sole and entire warranty pertaining to the product and is in lieu of and excludes all other warranties of any nature whatsoever, whether express, implied or arising by operation of law, including, but not limited to any implied warranties of merchantability or fitness for particular purpose. This warranty does not cover or provide for the reimbursement or payment of incidental or consequential damages.** Some states do not allow exclusion or limitations of incidental or consequential damages so the above limitation or exclusions may not apply if not allowed by state and local laws.

Any Items returned for repair or service must be sent shipping prepaid to an Authorized Serviced Center. **Shipping expense will be on the part of the owner to ship item for repairs.** Once the repairs are made the manufacturer will ship the item back to the owner at the manufacturer's expense (If within the continental US). **Innovative Concepts DOES NOT ship outside the Continental United State of America (CONUS). Shipping arrangements to and from the Authorized Serviced Center for individuals outside the CONUS - MUST be made before repairs are started. Innovative Concepts will not service any equipment until prior shipping arrangements are made.**

The Repair Center Duties: Will verify the unit is under warranty service agreement and conduct the following services. Will repair when possible or replace when necessary any Scan/Output Cable or Power Supply which does NOT meet the manufacturers standards. Will repair/replace any part of the product due to damage other than listed above. Will correct any defect and include the most current upgrades in the software programming, as well as perform other appropriate check/services.

Before any product is returned for warranty repair or out of warranty repair the sender must call The Main Distribution Center for a Return Merchandise Authorization Number (RMA#). Any product returned for warranty or non warranty repair must be delivered freight prepaid in either its original package or packing affording an equal degree of protection along with Power Supply and Scan/Output Cable. The "Warranty Repair Form" must be sent with the equipment at the time of repairs so technicians can troubleshoot and make the needed repair.

Please make a copy of this form for your records and mail the original form to the address below FOR THE WARRANTY TO BE ACTIVE -----DO NOT DELAY-----

Send Completed Form To:

A2 Service and Repair Center

3880 Stockton Hill Road

Ste. 103-132

Kingman, Az. 86409 USA

PLEASE PRINT CLEARLY

If we can not read your handwriting you will not be entered

into the computer. Take your time and make it clear.

A2 SERIAL NUMBER: _____ **AM3 SERIAL NUMBER:** _____

Distributor Name: _____ **Telephone #** (____)-(____) _____ **-** _____ **Date** ____/____/____

**** If your address is outside the USA please write the correct address format and information on the back of this form and mail in as normal. Thank you**

Name: _____

Address: _____

City: _____ **State:** _____ **Zip:** _____ - _____

Phone Number (____) _____ - _____ **Email address:** _____

What Innovative Concept products do you own?

_____ **Matrix M2 or AM3 System** _____ **A2 ABPA** _____ **EM Pulse** _____ **P2 Personal Pulses** _____ **Pen Armor**

This section must be completed and returned to Innovative Concepts at the address above for the warranty to be valid. We do not share or release any information given.